




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022820.D
 Acq On : 04 May 2022 23:26
 Operator : SY/VA
 Sample : N2699-06
 Misc : 4.76g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBQ9

Manual IntegrationsAPPROVED

Quant Time: May 05 03:00:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 05 02:23:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

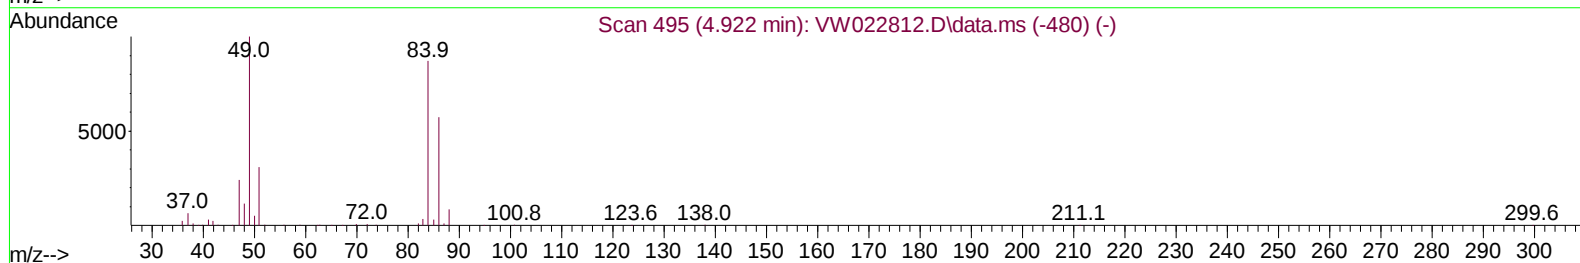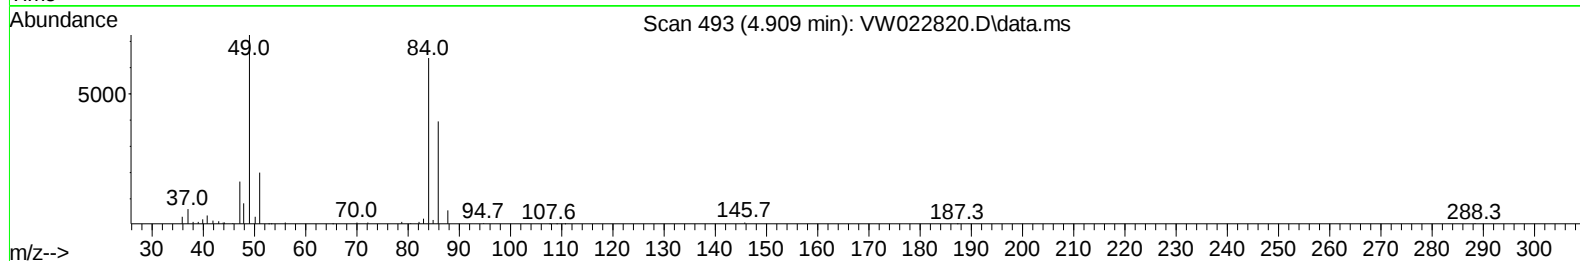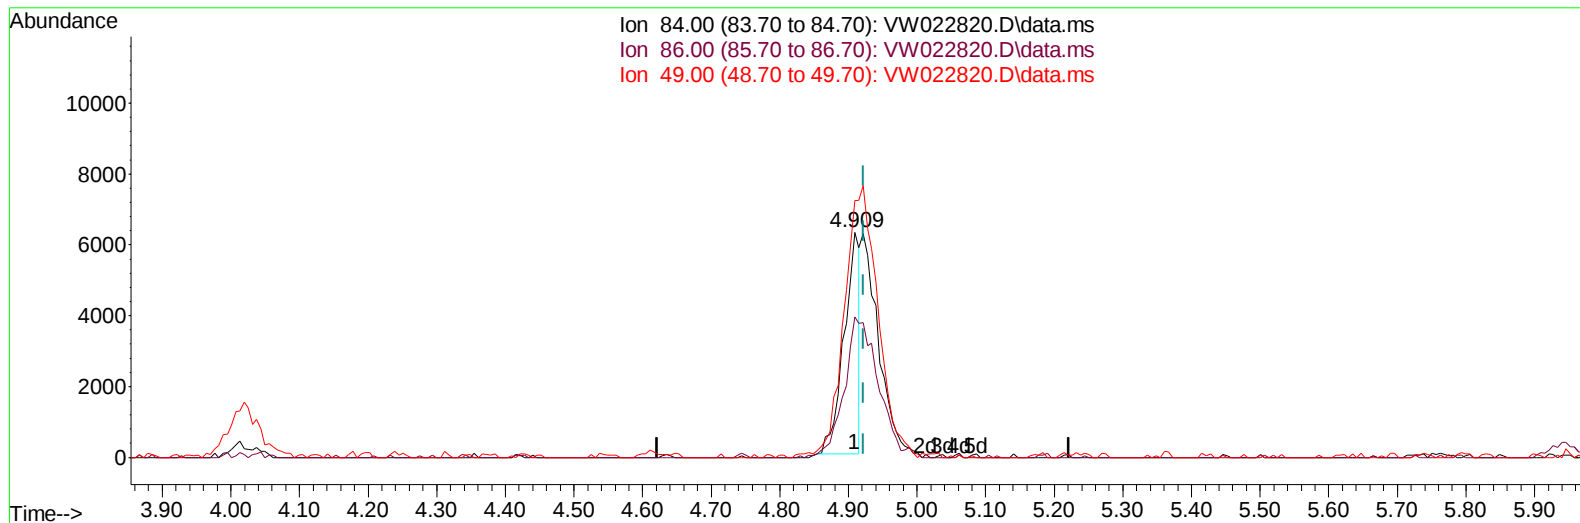

TIC: VW022820.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.012) 2.30 ug/L

response 9997

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.90	62.26
49.00	117.80	113.96
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022820.D
 Acq On : 04 May 2022 23:26
 Operator : SY/VA
 Sample : N2699-06
 Misc : 4.76g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBQ9

Manual IntegrationsAPPROVED

Quant Time: May 05 03:00:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 05 02:23:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

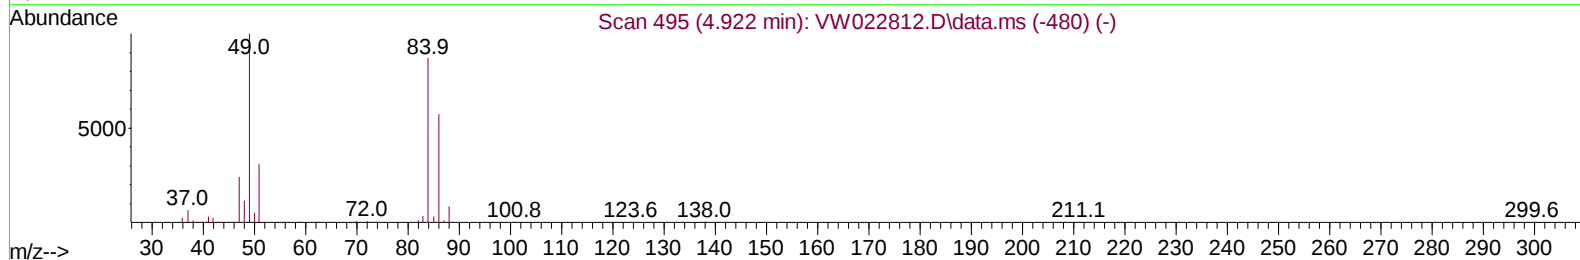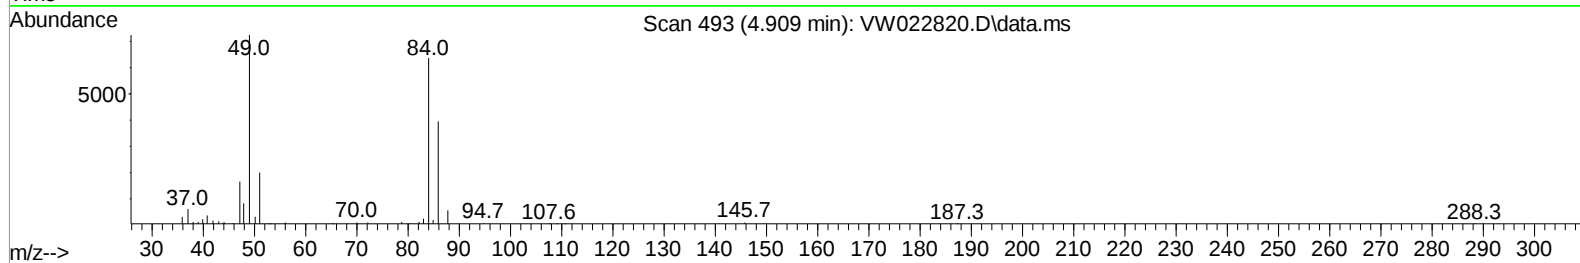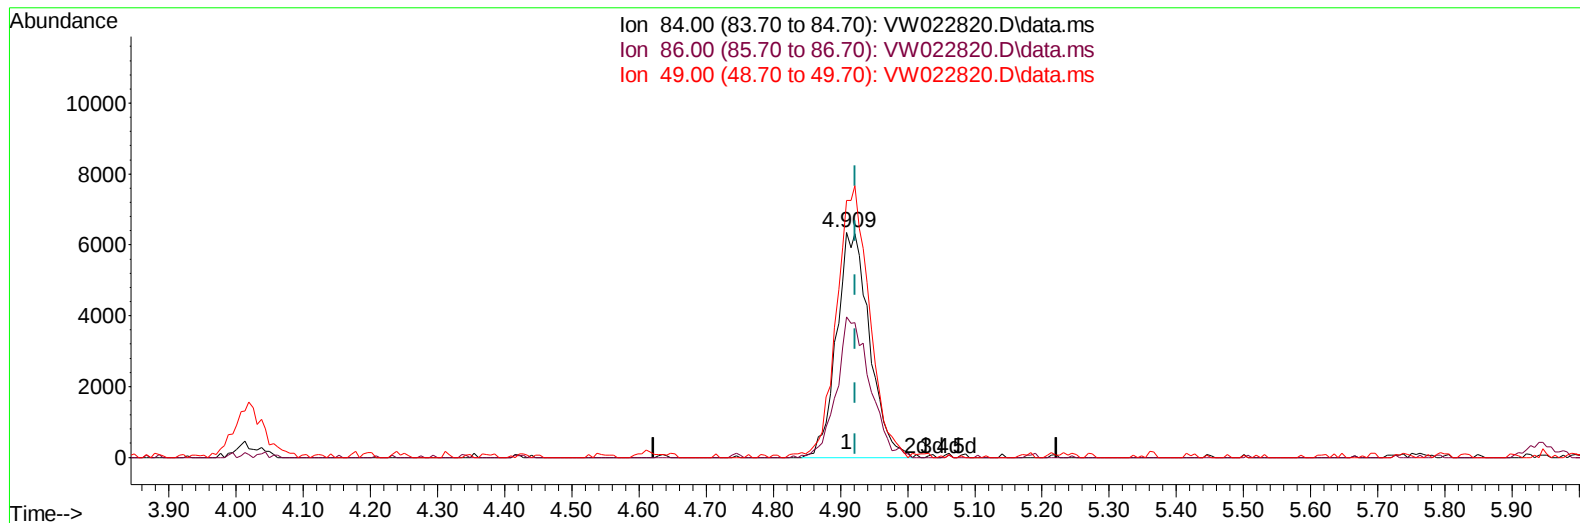

TIC: VW022820.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.012) 4.96 ug/L m

response 21608

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.90	62.26
49.00	117.80	113.96
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022820.D
 Acq On : 04 May 2022 23:26
 Operator : SY/VA
 Sample : N2699-06
 Misc : 4.76g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBQ9

Manual IntegrationsAPPROVED

Quant Time: May 05 03:00:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 05 02:23:51 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	297659	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	253976	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	94269	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	119205	19.520	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.080%	
7) Chloroethane-d5	2.885	69	88531	22.283	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	89.120%	
11) 1,1-Dichloroethene-d2	4.013	63	112116	14.208	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	56.840%	
21) 2-Butanone-d5	7.073	46	34459	29.677	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	59.360%	
24) Chloroform-d	7.647	84	198606	22.774	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.080%	
26) 1,2-Dichloroethane-d4	8.305	65	114795	24.001	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	96.000%	
32) Benzene-d6	8.274	84	367104	25.077	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	100.320%	
36) 1,2-Dichloropropane-d6	9.274	67	112732	27.414	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	109.640%	
41) Toluene-d8	10.323	98	313708	22.184	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	88.720%	
43) trans-1,3-Dichloroprop...	10.573	79	32723	17.283	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	69.120%	
47) 2-Hexanone-d5	10.926	63	28018	35.692	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	71.380%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	96339	25.135	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	100.560%	
66) 1,2-Dichlorobenzene-d4	13.853	152	77004	23.368	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	93.480%	
Target Compounds						
16) Methylene chloride	4.909	84	21608m	4.961	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022820.D
Acq On : 04 May 2022 23:26
Operator : SY/VA
Sample : N2699-06
Misc : 4.76g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGBQ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 05 03:00:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 05 02:23:51 2022
Response via : Initial Calibration

