

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022794.D
 Acq On : 04 May 2022 12:04
 Operator : SY/VA
 Sample : N2632-06RE
 Misc : 6.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A7RE

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/05/2022
 Supervised By : Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:35:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	271544	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	203365	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	58443	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	136387	24.481	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.920%		
7) Chloroethane-d5	2.885	69	95872	26.451	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	105.800%		
11) 1,1-Dichloroethene-d2	4.019	63	115719	16.075	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	64.320%		
21) 2-Butanone-d5	7.080	46	52919	49.959	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	99.920%		
24) Chloroform-d	7.647	84	194515	24.450	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	97.800%		
26) 1,2-Dichloroethane-d4	8.305	65	107412	24.617	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	98.480%		
32) Benzene-d6	8.274	84	364433	31.090	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	124.360%		
36) 1,2-Dichloropropane-d6	9.274	67	108271	32.882	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	131.520%#		
41) Toluene-d8	10.323	98	292091	25.795	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	103.200%		
43) trans-1,3-Dichloroprop...	10.579	79	33353	21.999	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.000%		
47) 2-Hexanone-d5	10.920	63	37813	60.157	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	120.320%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	90640	29.534	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	118.120%		
66) 1,2-Dichlorobenzene-d4	13.853	152	63924	31.290	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	125.160%#		
Target Compounds					Qvalue	
13) Acetone	4.135	43	3575m	4.508	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022794.D
Acq On : 04 May 2022 12:04
Operator : SY/VA
Sample : N2632-06RE
Misc : 6.80g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW4A7RE

Quant Time: May 04 23:35:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

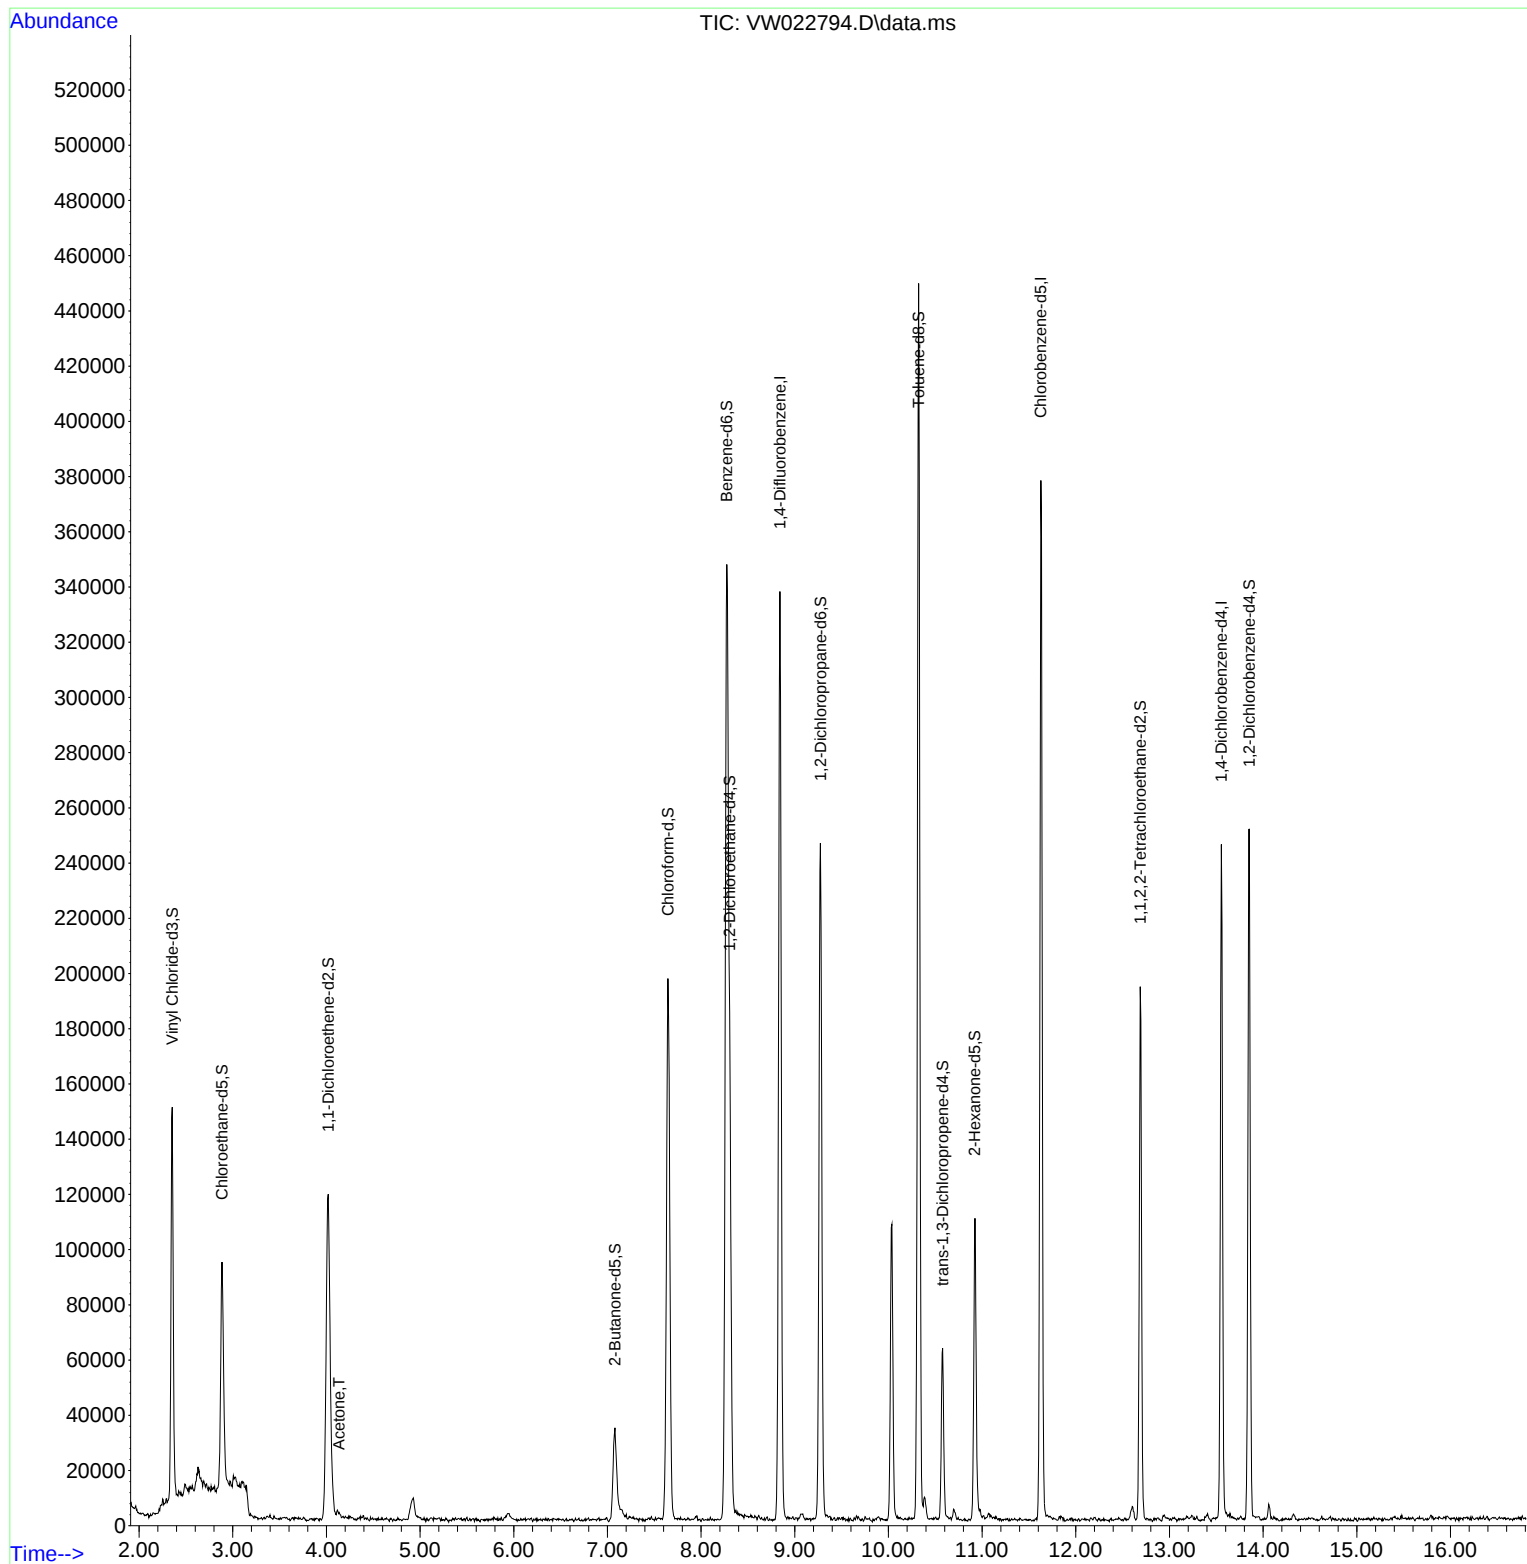

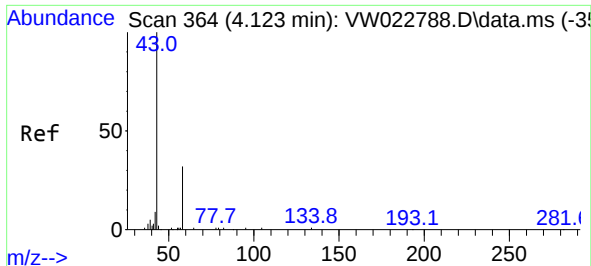

#13
Acetone
Concen: 4.508 ug/L m
RT: 4.135 min Scan# 30
Delta R.T. 0.012 min
Lab File: VW022794.D
Acq: 04 May 2022 12:04

Instrument :
MSVOA_W
ClientSampleId :
EW4A7RE

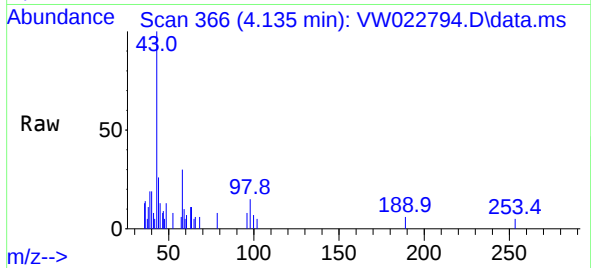

Tgt Ion: 43 Resp: 3579
Ion Ratio Lower Upper
43 100
58 5.9 0.0 64.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

