

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022799.D
 Acq On : 04 May 2022 14:05
 Operator : SY/VA
 Sample : N2632-14RE
 Misc : 7.66g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B6RE

Quant Time: May 04 23:36:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	273750	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	174413	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	33126	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.355	65	140754	25.061	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.240%	
7) Chloroethane-d5		2.885	69	101584	27.801	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.200%	
11) 1,1-Dichloroethene-d2		4.013	63	124033	17.091	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.360%	
21) 2-Butanone-d5		7.074	46	55650	52.114	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.220%	
24) Chloroform-d		7.647	84	200225	24.965	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.840%	
26) 1,2-Dichloroethane-d4		8.305	65	109543	24.903	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.600%	
32) Benzene-d6		8.275	84	368445	36.650	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	146.600%#	
36) 1,2-Dichloropropane-d6		9.275	67	108366	38.374	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	153.480%#	
41) Toluene-d8		10.323	98	271133	27.919	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	111.680%	
43) trans-1,3-Dichloroprop...		10.579	79	30013	23.082	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.320%	
47) 2-Hexanone-d5		10.921	63	36962	68.565	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	137.120%#	
56) 1,1,2,2-Tetrachloroeth...		12.689	84	82905	31.498	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	126.000%#	
66) 1,2-Dichlorobenzene-d4		13.853	152	34901	30.140	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	120.560%#	
Target Compounds							
13) Acetone		4.129	43	4572	5.719	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022799.D
Acq On : 04 May 2022 14:05
Operator : SY/VA
Sample : N2632-14RE
Misc : 7.66g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4B6RE


Quant Time: May 04 23:36:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

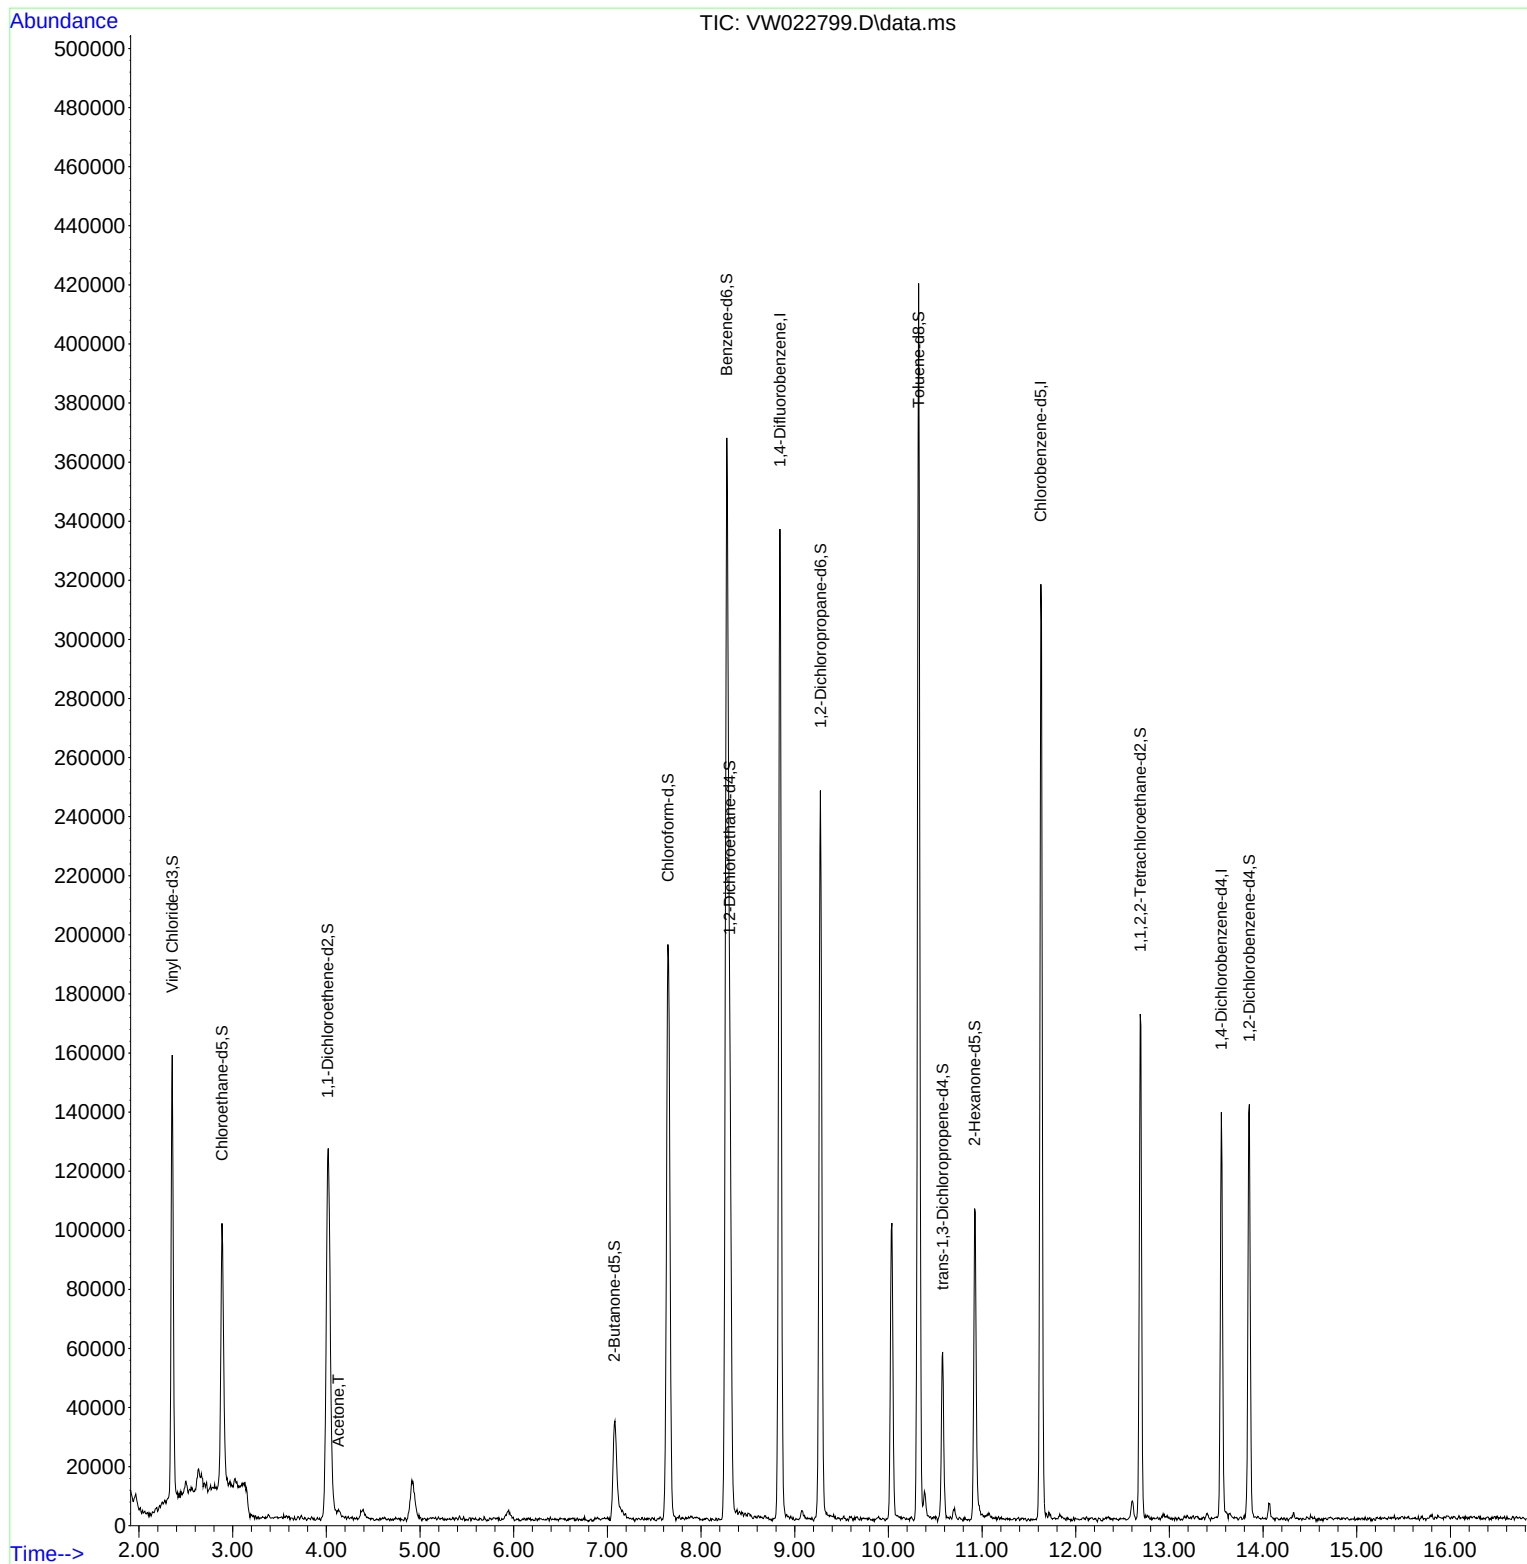

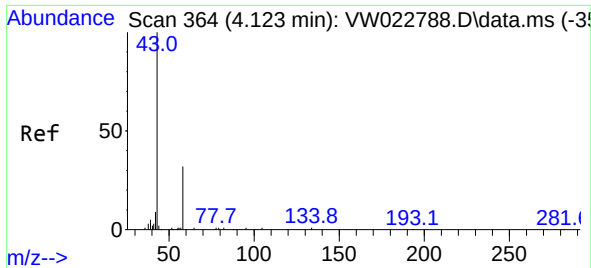

#13
 Acetone
 Concen: 5.719 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022799.D
 Acq: 04 May 2022 14:05

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B6RE

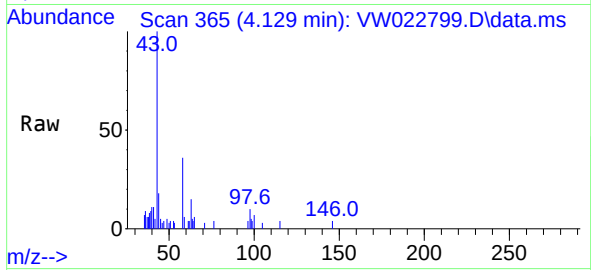

Tgt Ion: 43 Resp: 4572
 Ion Ratio Lower Upper
 43 100
 58 30.5 0.0 64.0

