

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022800.D
 Acq On : 04 May 2022 14:29
 Operator : SY/VA
 Sample : N2632-15RE
 Misc : 7.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B7RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:36:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	281042	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	182182	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	36450	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	149925	26.002	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	104.000%	
7) Chloroethane-d5	2.885	69	108122	28.823	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	115.280%	
11) 1,1-Dichloroethene-d2	4.013	63	129438	17.374	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	69.480%	
21) 2-Butanone-d5	7.074	46	60848	55.503	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	111.000%	
24) Chloroform-d	7.647	84	212158	25.766	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	103.080%	
26) 1,2-Dichloroethane-d4	8.305	65	113590	25.153	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	100.600%	
32) Benzene-d6	8.275	84	387217	36.875	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	147.480%#	
36) 1,2-Dichloropropane-d6	9.274	67	114826	38.928	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	155.720%#	
41) Toluene-d8	10.323	98	295256	29.107	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	116.440%	
43) trans-1,3-Dichloroprop...	10.579	79	33383	24.579	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	98.320%	
47) 2-Hexanone-d5	10.920	63	40214	71.416	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	142.840%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	86465	31.449	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	125.800%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	38483	30.202	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	120.800%#	
Target Compounds					Qvalue	
13) Acetone	4.123	43	3952m	4.815	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022800.D
Acq On : 04 May 2022 14:29
Operator : SY/VA
Sample : N2632-15RE
Misc : 7.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW4B7RE

Quant Time: May 04 23:36:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 05/05/2022
Supervised By : Mahesh Dadoda 05/09/2022

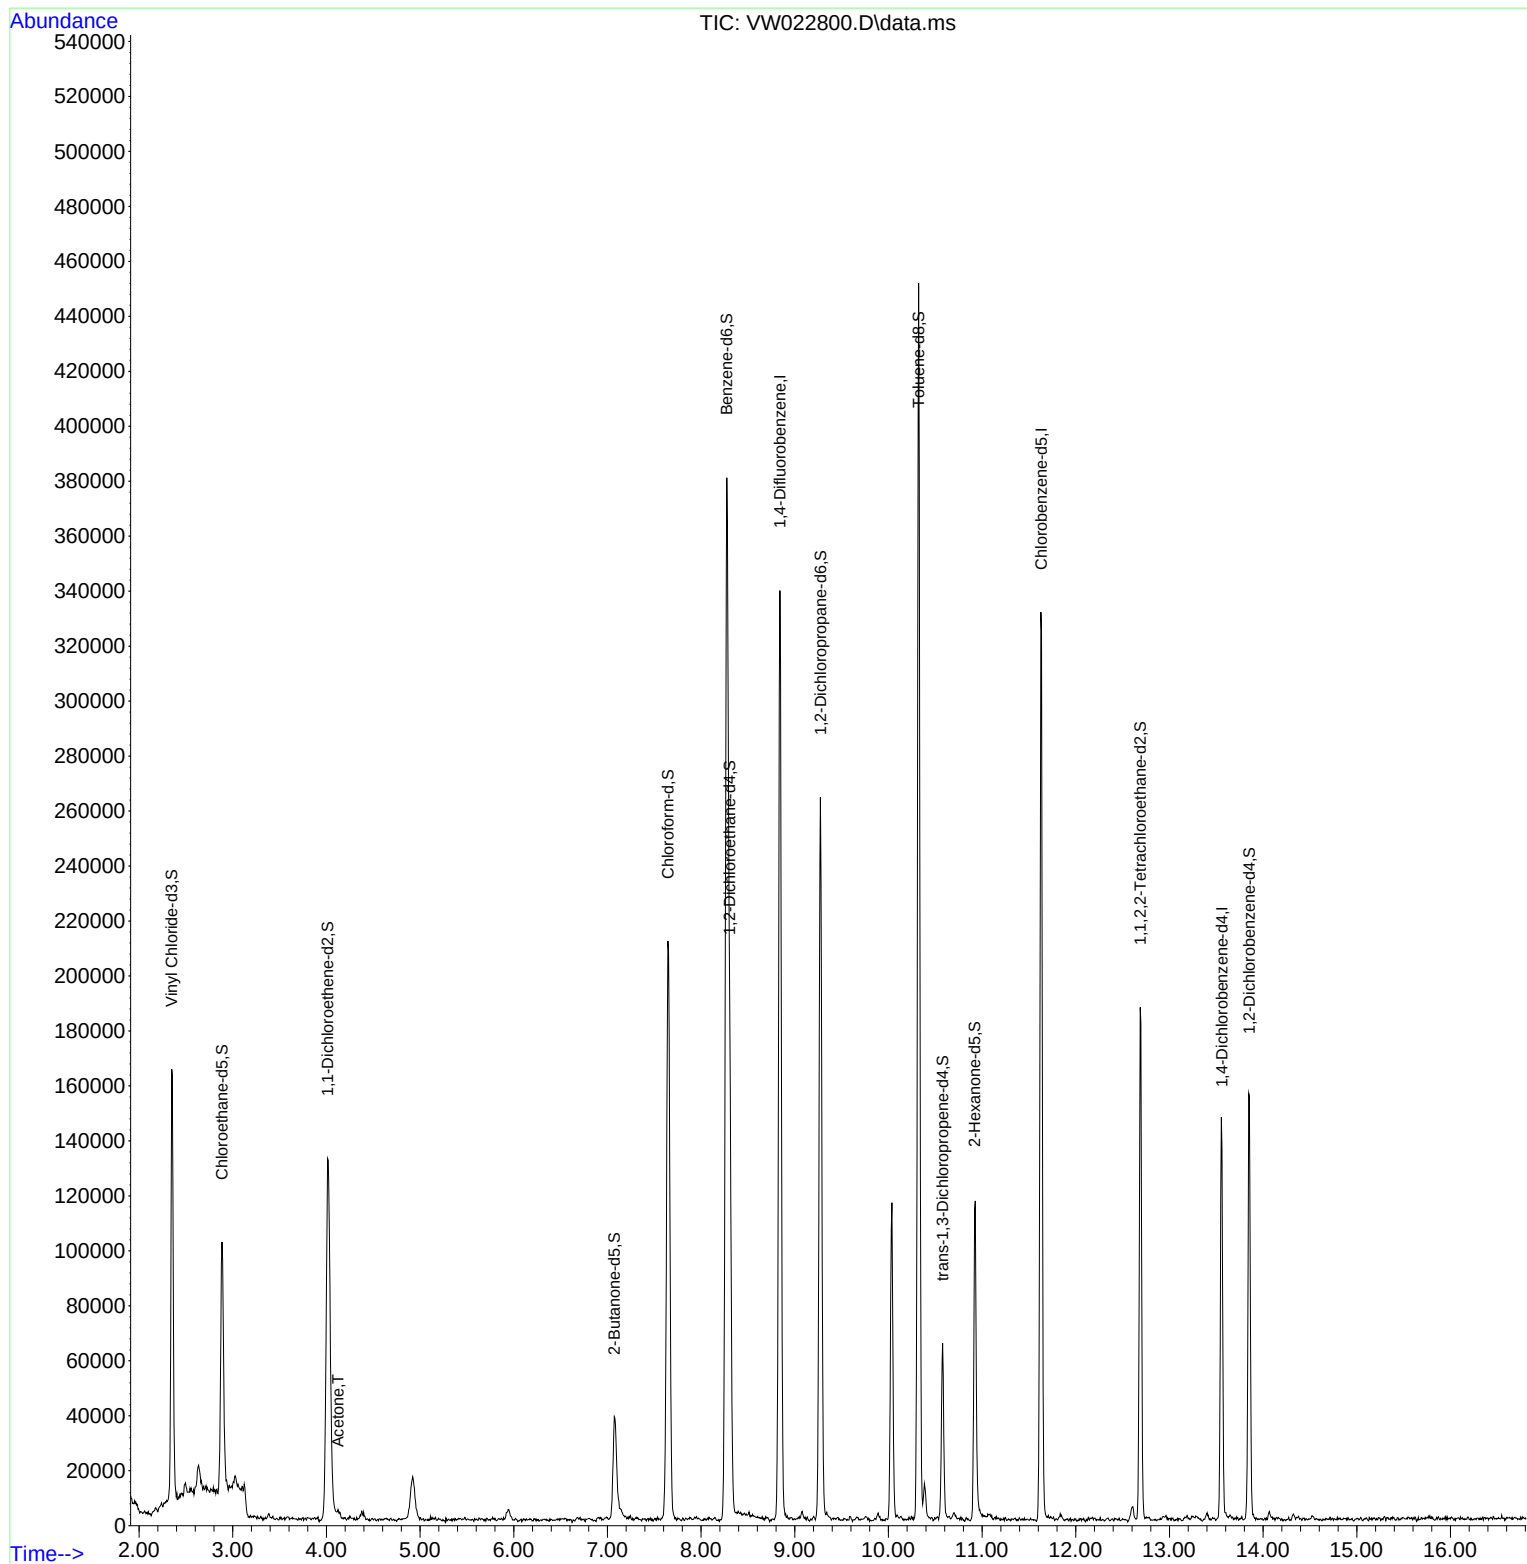

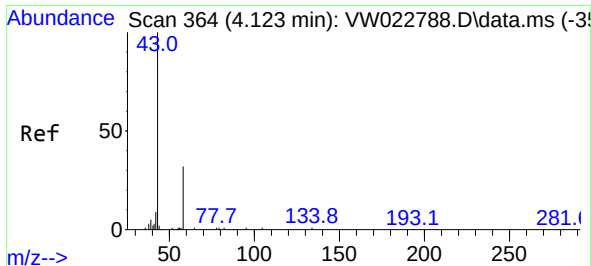

#13
Acetone
Concen: 4.815 ug/L m
RT: 4.123 min Scan# 30
Delta R.T. 0.000 min
Lab File: VW022800.D
Acq: 04 May 2022 14:29

Instrument :
MSVOA_W
ClientSampleId :
EW4B7RE

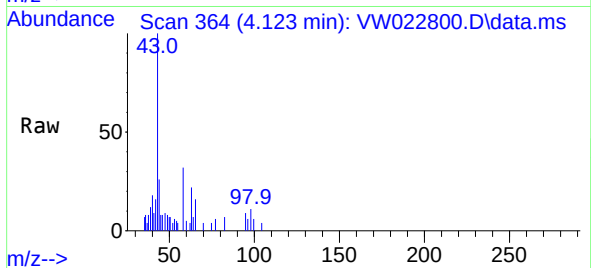

Tgt Ion: 43 Resp: 3952
Ion Ratio Lower Upper
43 100
58 33.5 0.0 64.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

