

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022811.D
 Acq On : 04 May 2022 18:54
 Operator : SY/VA
 Sample : N2638-02
 Misc : 5.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXKZ3

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/05/2022
 Supervised By : Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:38:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	340343	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	322645	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	156269	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	137028	19.624	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.480%
7) Chloroethane-d5	2.885	69	99303	21.860	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.440%
11) 1,1-Dichloroethene-d2	4.013	63	124051	13.749	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.000%
21) 2-Butanone-d5	7.080	46	54316	40.912	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.820%
24) Chloroform-d	7.647	84	210058	21.066	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.280%
26) 1,2-Dichloroethane-d4	8.305	65	120344	22.005	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.040%
32) Benzene-d6	8.275	84	402457	21.641	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.560%
36) 1,2-Dichloropropane-d6	9.274	67	121978	23.350	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.400%
41) Toluene-d8	10.323	98	372595	20.740	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.960%
43) trans-1,3-Dichloroprop...	10.579	79	46200	19.207	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.840%
47) 2-Hexanone-d5	10.927	63	43310	43.430	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.860%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	101041	20.752	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.000%
66) 1,2-Dichlorobenzene-d4	13.853	152	110230	20.179	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.720%
Target Compounds					Qvalue	
13) Acetone	4.129	43	6125m	6.162	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022811.D
Acq On : 04 May 2022 18:54
Operator : SY/VA
Sample : N2638-02
Misc : 5.40g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EXKZ3

Quant Time: May 04 23:38:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 05/05/2022
Supervised By : Mahesh Dadoda 05/09/2022

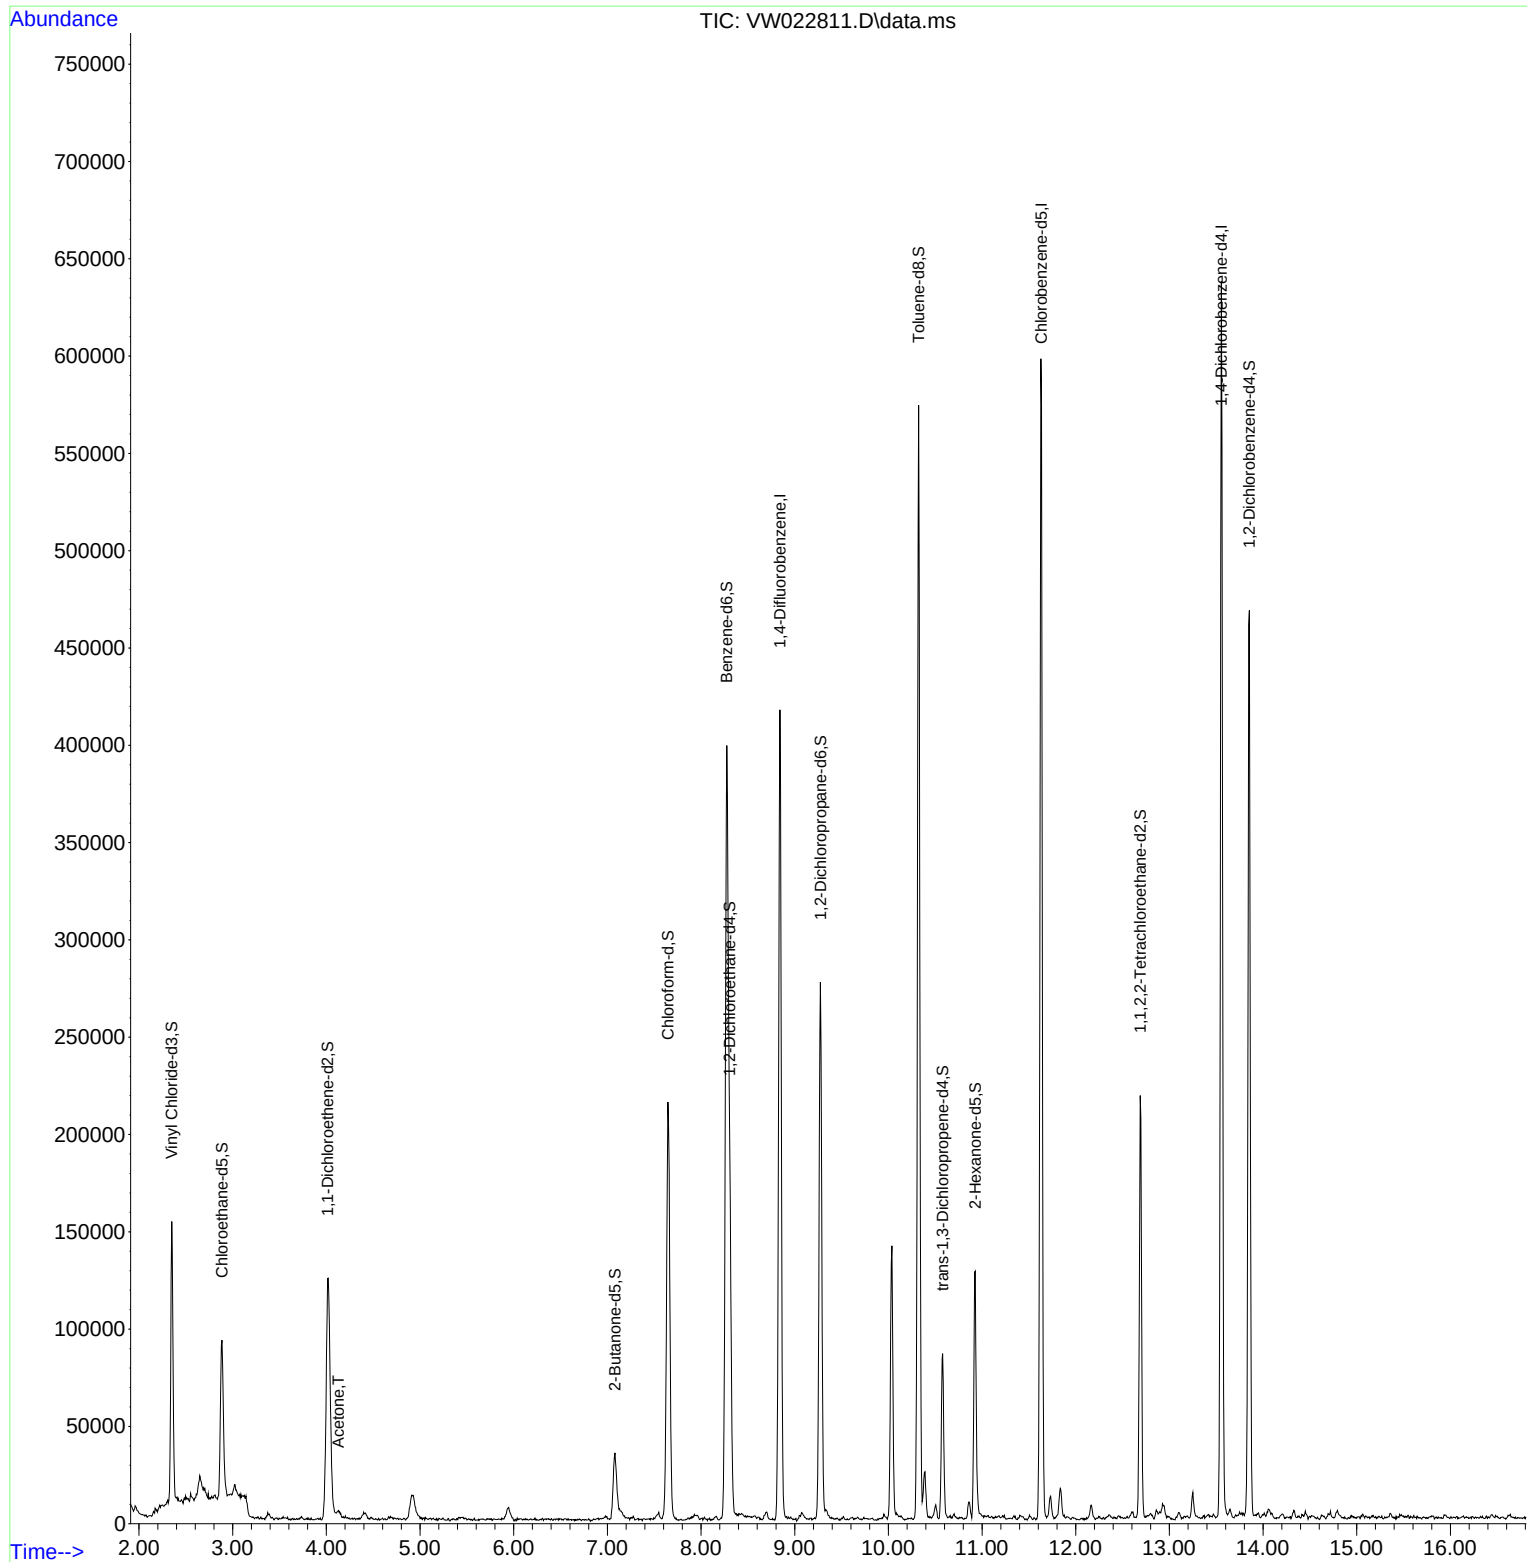

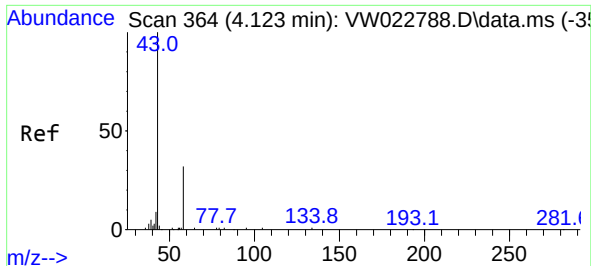

#13
Acetone
Concen: 6.162 ug/L m
RT: 4.129 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW022811.D
Acq: 04 May 2022 18:54

Instrument :
MSVOA_W
ClientSampleId :
EXKZ3

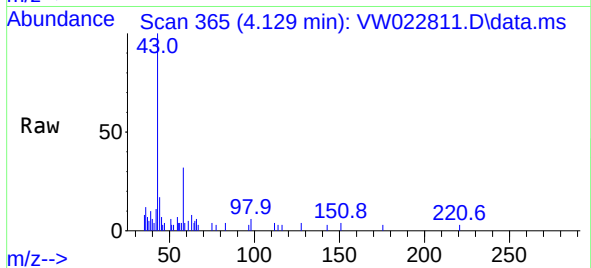

Tgt Ion: 43 Resp: 6125
Ion Ratio Lower Upper
43 100
58 14.2 0.0 64.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

