

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022824.D
 Acq On : 05 May 2022 01:02
 Operator : SY/VA
 Sample : N2699-09
 Misc : 5.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBR2

Quant Time: May 05 03:00:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 05 02:23:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	269204	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	225403	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	75009	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	112657	20.397	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.600%
7) Chloroethane-d5	2.885	69	79607	22.155	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.600%
11) 1,1-Dichloroethene-d2	4.019	63	103204	14.461	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.840%
21) 2-Butanone-d5	7.074	46	25068	23.872	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	47.740%
24) Chloroform-d	7.653	84	185713	23.547	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.200%
26) 1,2-Dichloroethane-d4	8.305	65	106934	24.720	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.880%
32) Benzene-d6	8.275	84	336840	25.927	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.720%
36) 1,2-Dichloropropane-d6	9.275	67	104175	28.545	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	114.160%
41) Toluene-d8	10.323	98	278552	22.195	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.760%
43) trans-1,3-Dichloroprop...	10.579	79	25838	15.376	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	61.520%
47) 2-Hexanone-d5	10.927	63	19981	28.680	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	57.360%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	85995	25.281	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	61856	23.591	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.360%
Target Compounds						Qvalue
16) Methylene chloride	4.916	84	19960	5.067	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022824.D
Acq On : 05 May 2022 01:02
Operator : SY/VA
Sample : N2699-09
Misc : 5.12g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGBR2

Quant Time: May 05 03:00:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 05 02:23:51 2022
Response via : Initial Calibration

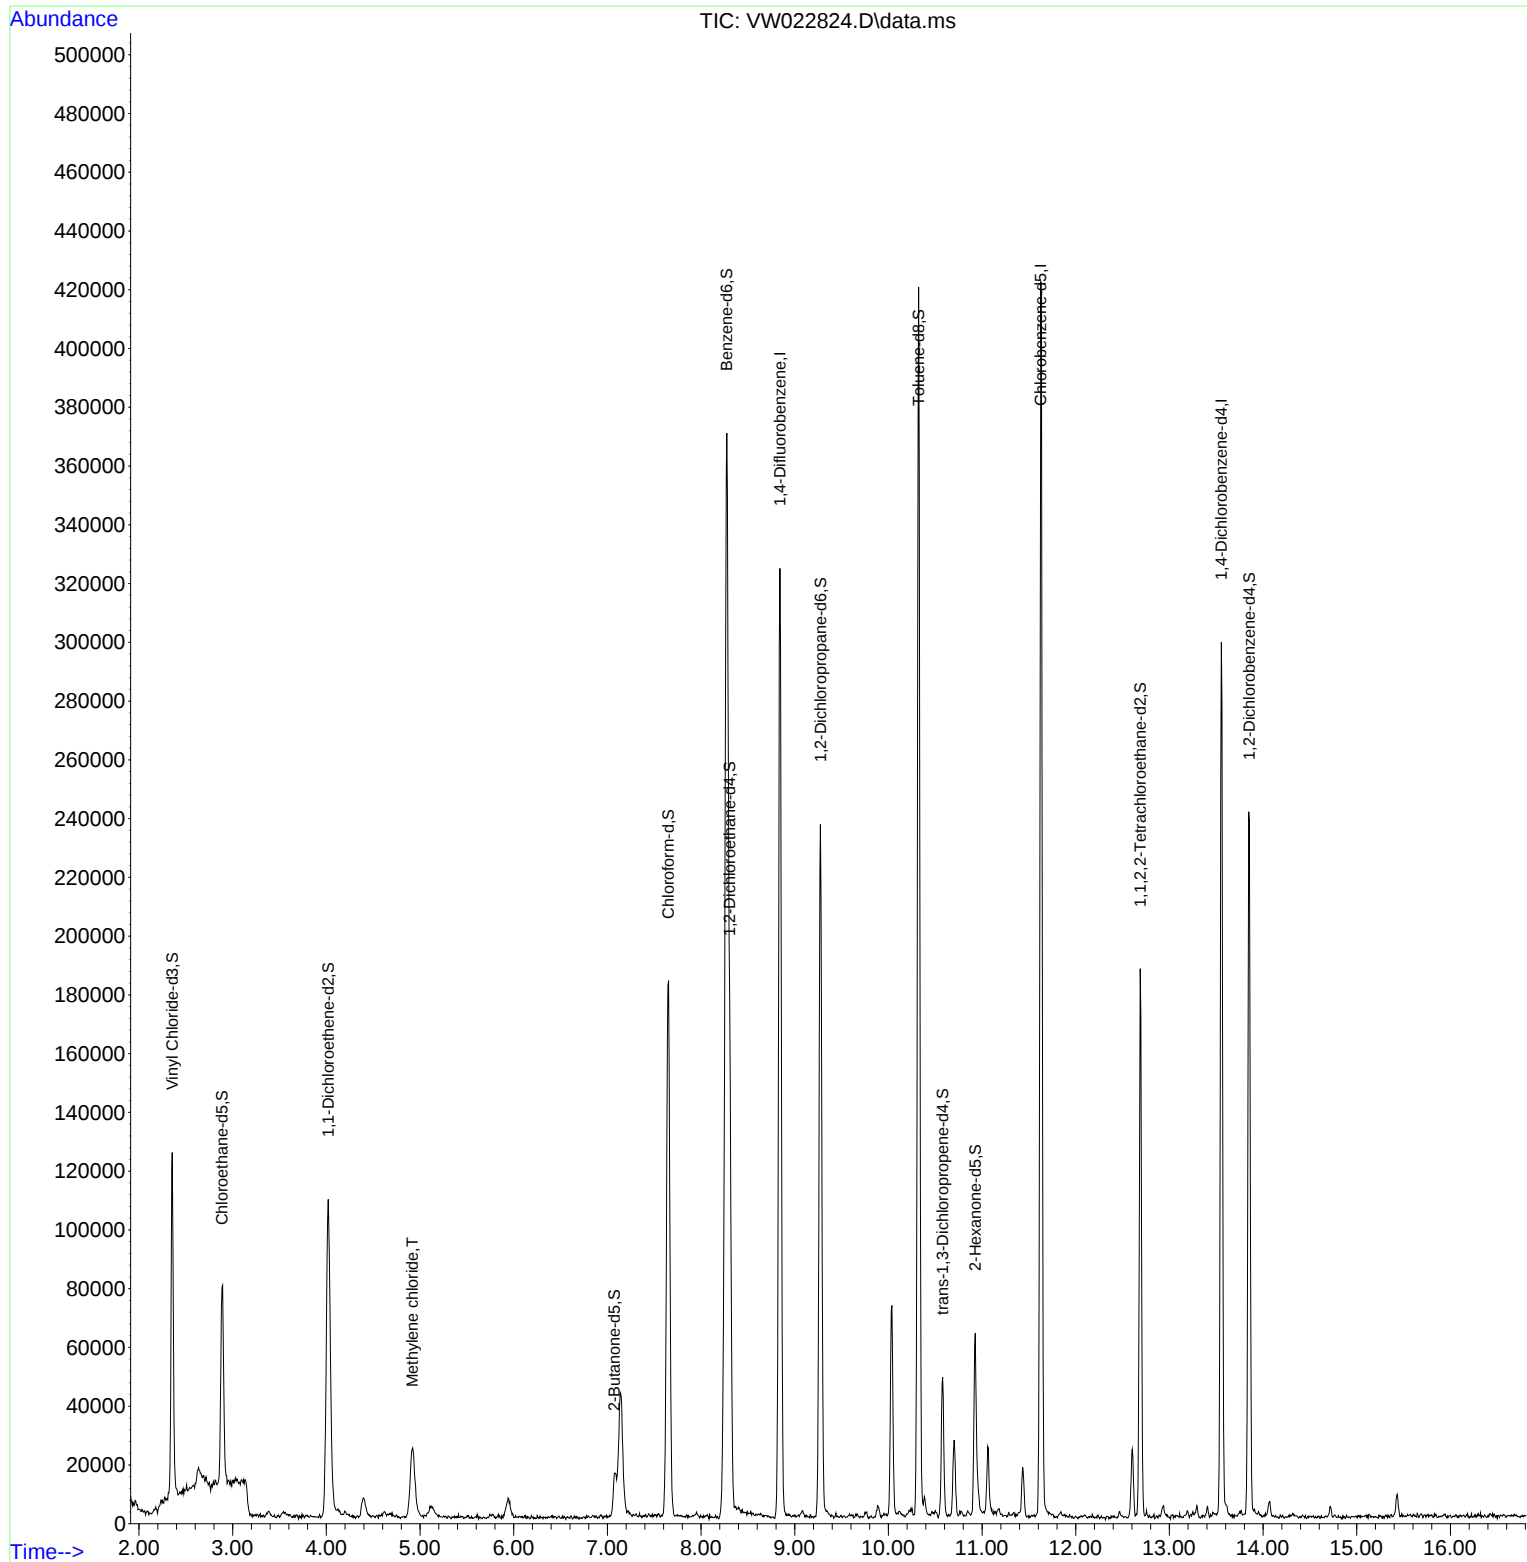

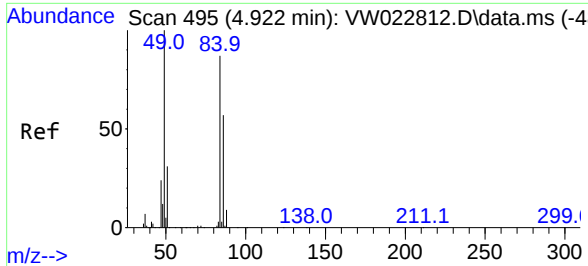

#16
Methylene chloride
Concen: 5.067 ug/L
RT: 4.916 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW022824.D
Acq: 05 May 2022 01:02

Instrument :
MSVOA_W
ClientSampleId :
BGBR2

Tgt Ion: 84 Resp: 19960

Ion	Ratio	Lower	Upper
84	100		
86	58.5	45.4	84.4
49	101.8	82.5	153.1

