

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022825.D
 Acq On : 05 May 2022 01:27
 Operator : SY/VA
 Sample : VIBLK448
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK448

Quant Time: May 05 03:01:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 05 02:23:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	280607	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	277897	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	135833	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	135438	23.526	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.120%
7) Chloroethane-d5	2.885	69	96577	25.785	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.160%
11) 1,1-Dichloroethene-d2	4.013	63	126172	16.961	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.840%
21) 2-Butanone-d5	7.080	46	53601	48.969	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.940%
24) Chloroform-d	7.647	84	204872	24.920	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.680%
26) 1,2-Dichloroethane-d4	8.305	65	116658	25.872	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.480%
32) Benzene-d6	8.275	84	404105	25.228	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.920%
36) 1,2-Dichloropropane-d6	9.274	67	115304	25.626	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.520%
41) Toluene-d8	10.323	98	376909	24.359	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.440%
43) trans-1,3-Dichloroprop...	10.573	79	44636	21.545	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.200%
47) 2-Hexanone-d5	10.921	63	42155	49.078	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.160%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103350	24.644	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	120240	25.323	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.280%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	17697	4.310	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022825.D
Acq On : 05 May 2022 01:27
Operator : SY/VA
Sample : VIBLK448
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK448


Quant Time: May 05 03:01:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 05 02:23:51 2022
Response via : Initial Calibration

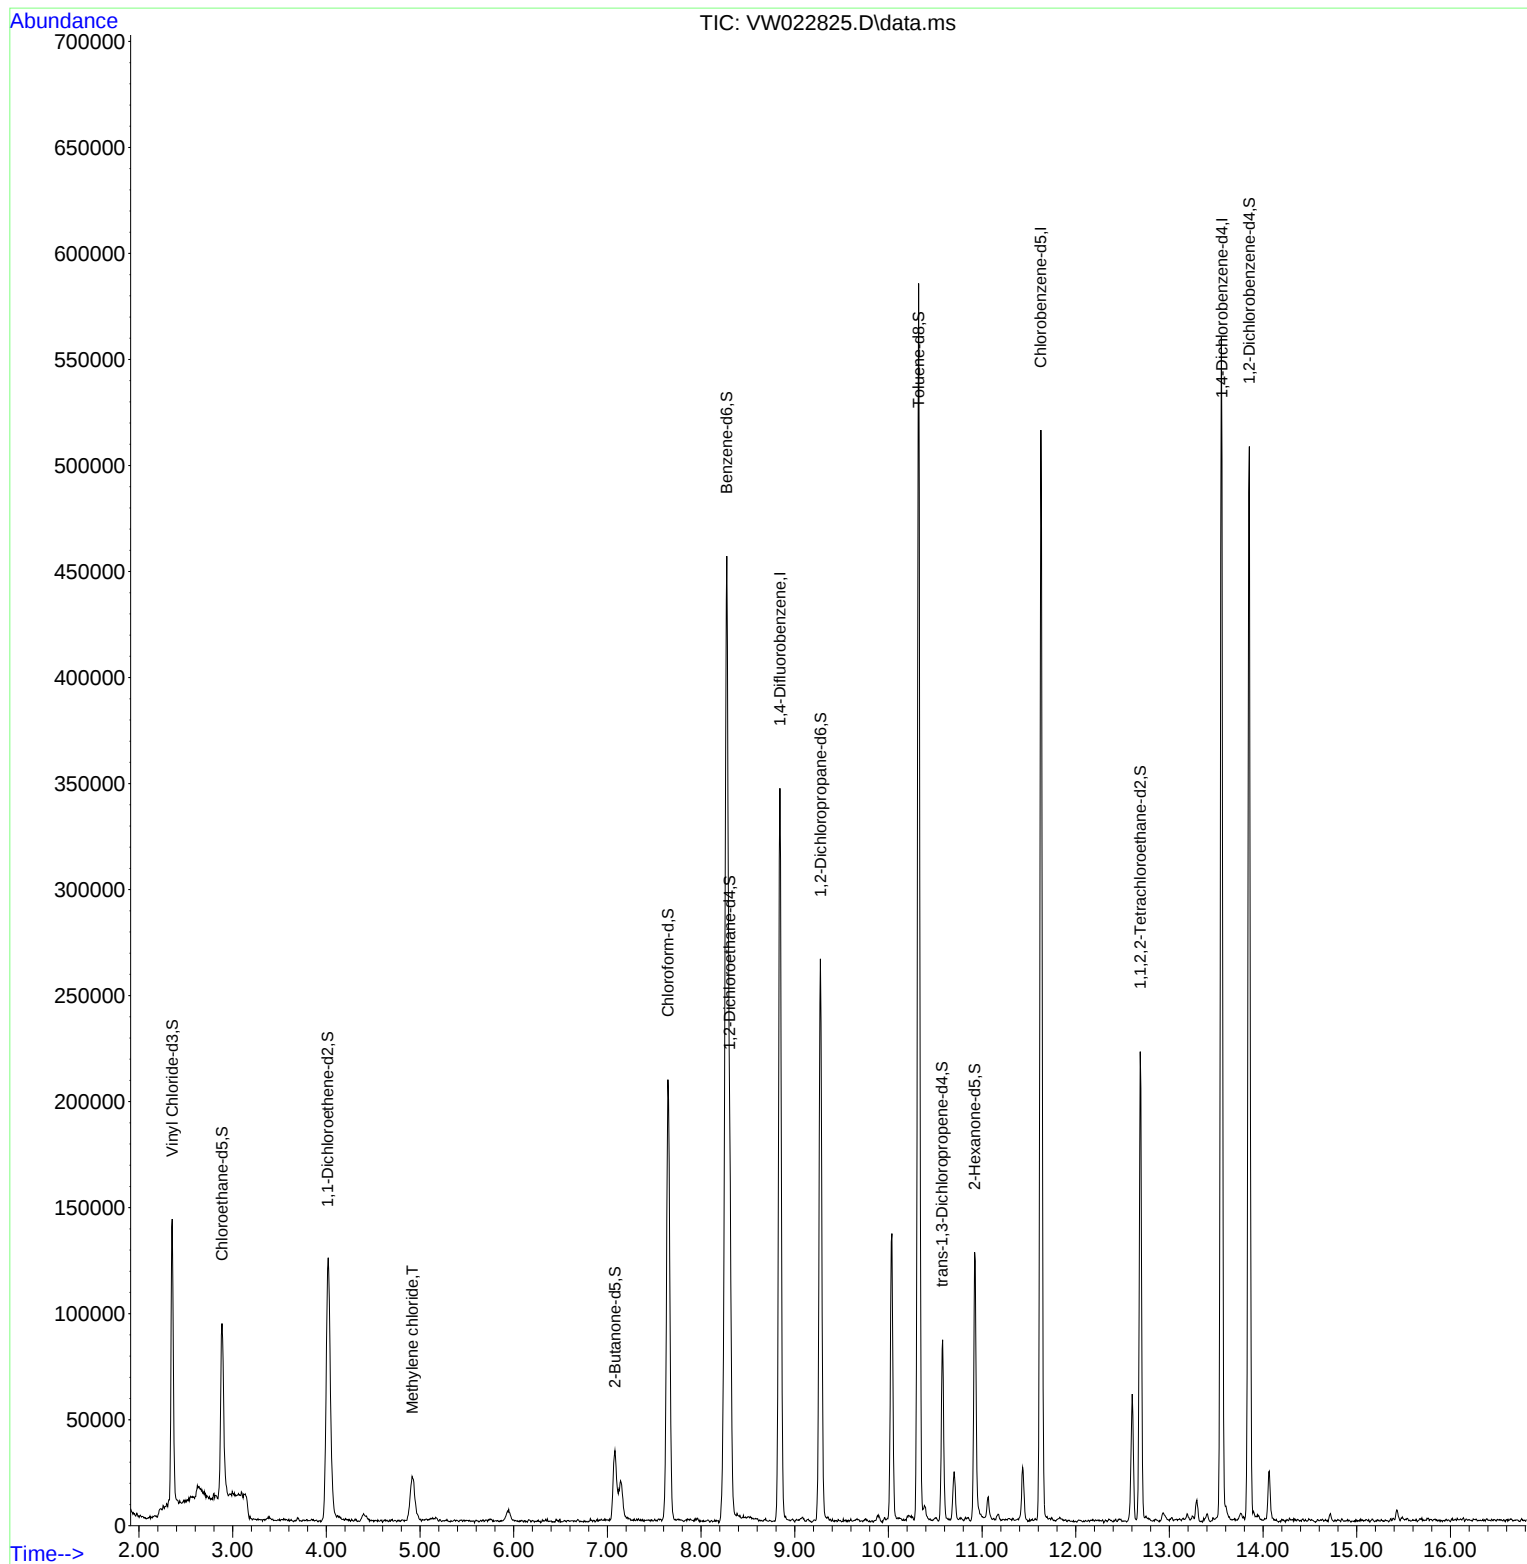

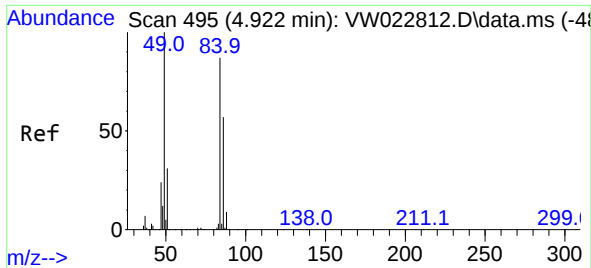

#16
Methylene chloride
Concen: 4.310 ug/L
RT: 4.915 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW022825.D
Acq: 05 May 2022 01:27

Instrument :
MSVOA_W
ClientSampleId :
VIBLK448

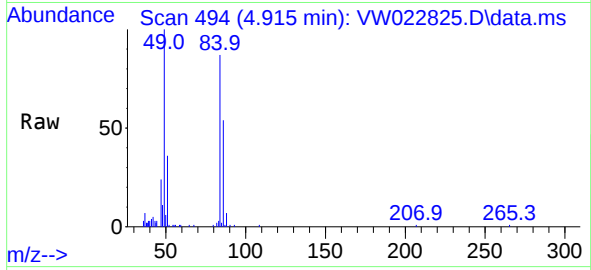

Tgt Ion: 84 Resp: 17697

Ion	Ratio	Lower	Upper
84	100		
86	61.7	45.4	84.4
49	114.4	82.5	153.1

