

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022827.D
 Acq On : 05 May 2022 02:15
 Operator : SY/VA
 Sample : N2699-11
 Misc : 4.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBR4

Quant Time: May 05 03:01:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 05 02:23:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	253499	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	208011	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	68019	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	107559	20.681	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.720%
7) Chloroethane-d5	2.885	69	79238	23.418	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.680%
11) 1,1-Dichloroethene-d2	4.019	63	95877	14.267	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.080%
21) 2-Butanone-d5	7.074	46	24809	25.089	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	50.180%
24) Chloroform-d	7.647	84	169285	22.793	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.160%
26) 1,2-Dichloroethane-d4	8.305	65	99998	24.549	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.200%
32) Benzene-d6	8.275	84	300696	25.080	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.320%
36) 1,2-Dichloropropane-d6	9.275	67	95659	28.403	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.600%
41) Toluene-d8	10.323	98	247762	21.392	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.560%
43) trans-1,3-Dichloroprop...	10.579	79	23108	14.901	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	59.600%
47) 2-Hexanone-d5	10.927	63	19999	31.106	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.220%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	82853	26.394	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	58080	24.427	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.720%
Target Compounds						Qvalue
16) Methylene chloride	4.922	84	19151	5.163	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022827.D
Acq On : 05 May 2022 02:15
Operator : SY/VA
Sample : N2699-11
Misc : 4.29g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGBR4


Quant Time: May 05 03:01:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 05 02:23:51 2022
Response via : Initial Calibration

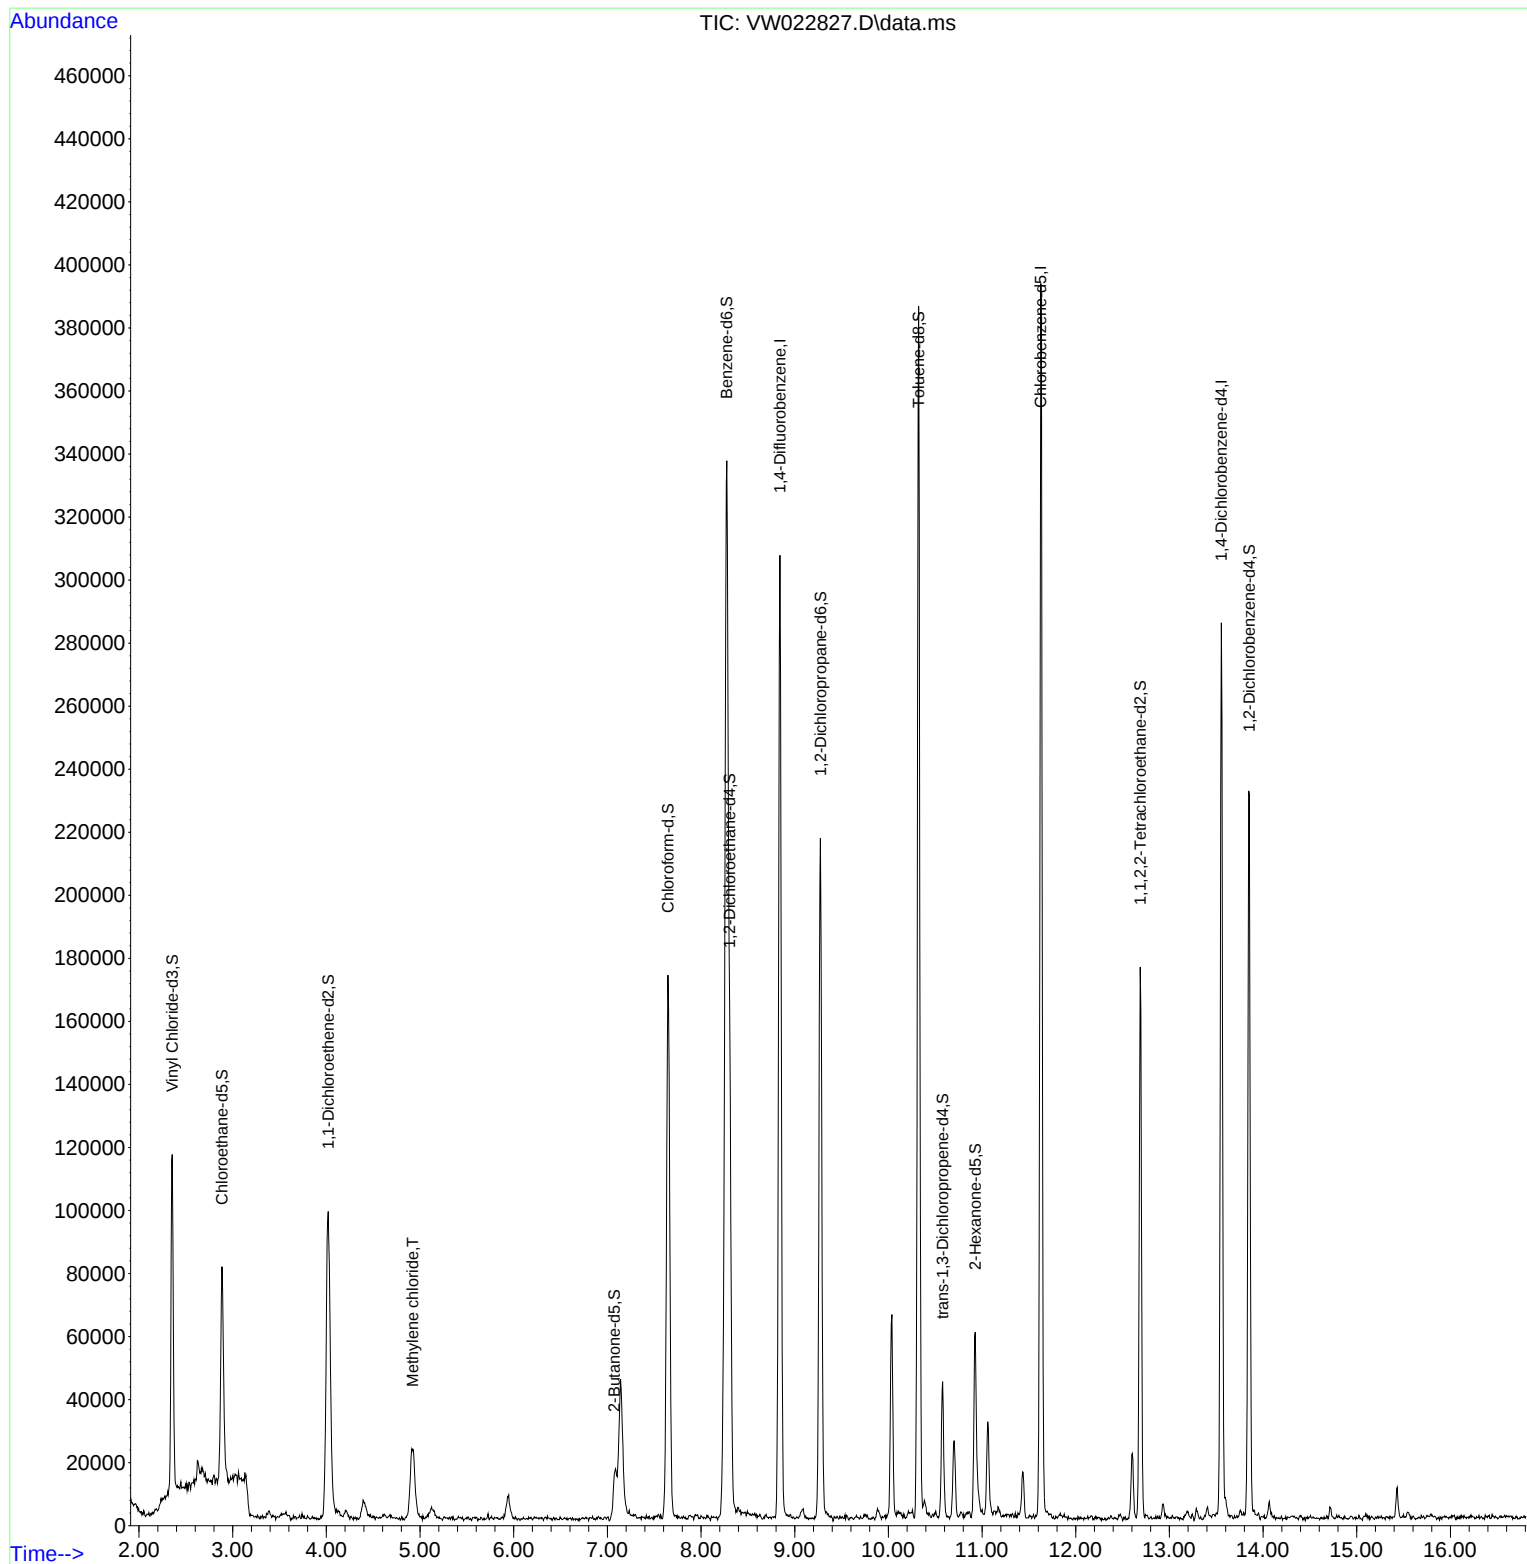

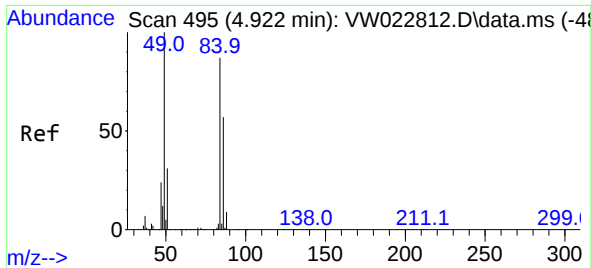

#16
Methylene chloride
Concen: 5.163 ug/L
RT: 4.922 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW022827.D
Acq: 05 May 2022 02:15

Instrument :
MSVOA_W
ClientSampleId :
BGBR4

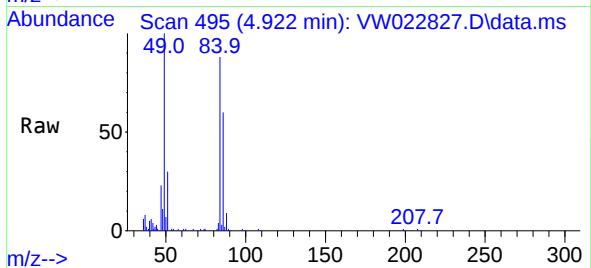

Tgt Ion:	84	Resp:	19151
Ion	Ratio	Lower	Upper
84	100		
86	68.1	45.4	84.4
49	113.7	82.5	153.1

