

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022835.D
 Acq On : 05 May 2022 12:24
 Operator : SY/VA
 Sample : N2699-04RE
 Misc : 4.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBQ7

Quant Time: May 06 01:06:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 01:05:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	349612	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	303708	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	114705	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	145295	20.256	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.040%
7) Chloroethane-d5	2.885	69	102192	21.899	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.600%
11) 1,1-Dichloroethene-d2	4.013	63	140158	15.123	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.480%
21) 2-Butanone-d5	7.080	46	47177	34.593	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.180%
24) Chloroform-d	7.653	84	230204	22.475	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.880%
26) 1,2-Dichloroethane-d4	8.305	65	126488	22.516	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.080%
32) Benzene-d6	8.275	84	436652	24.944	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.760%
36) 1,2-Dichloropropane-d6	9.275	67	128723	26.177	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.720%
41) Toluene-d8	10.323	98	388988	23.003	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.000%
43) trans-1,3-Dichloroprop...	10.579	79	43251	19.103	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.400%
47) 2-Hexanone-d5	10.921	63	36398	38.774	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.540%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	99305	21.667	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.680%
66) 1,2-Dichlorobenzene-d4	13.853	152	85373	21.292	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.160%
Target Compounds					Qvalue	
13) Acetone	4.129	43	9049	8.862	ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
Data File : VW022835.D
Acq On : 05 May 2022 12:24
Operator : SY/VA
Sample : N2699-04RE
Misc : 4.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGBQ7

Quant Time: May 06 01:06:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 06 01:05:05 2022
Response via : Initial Calibration

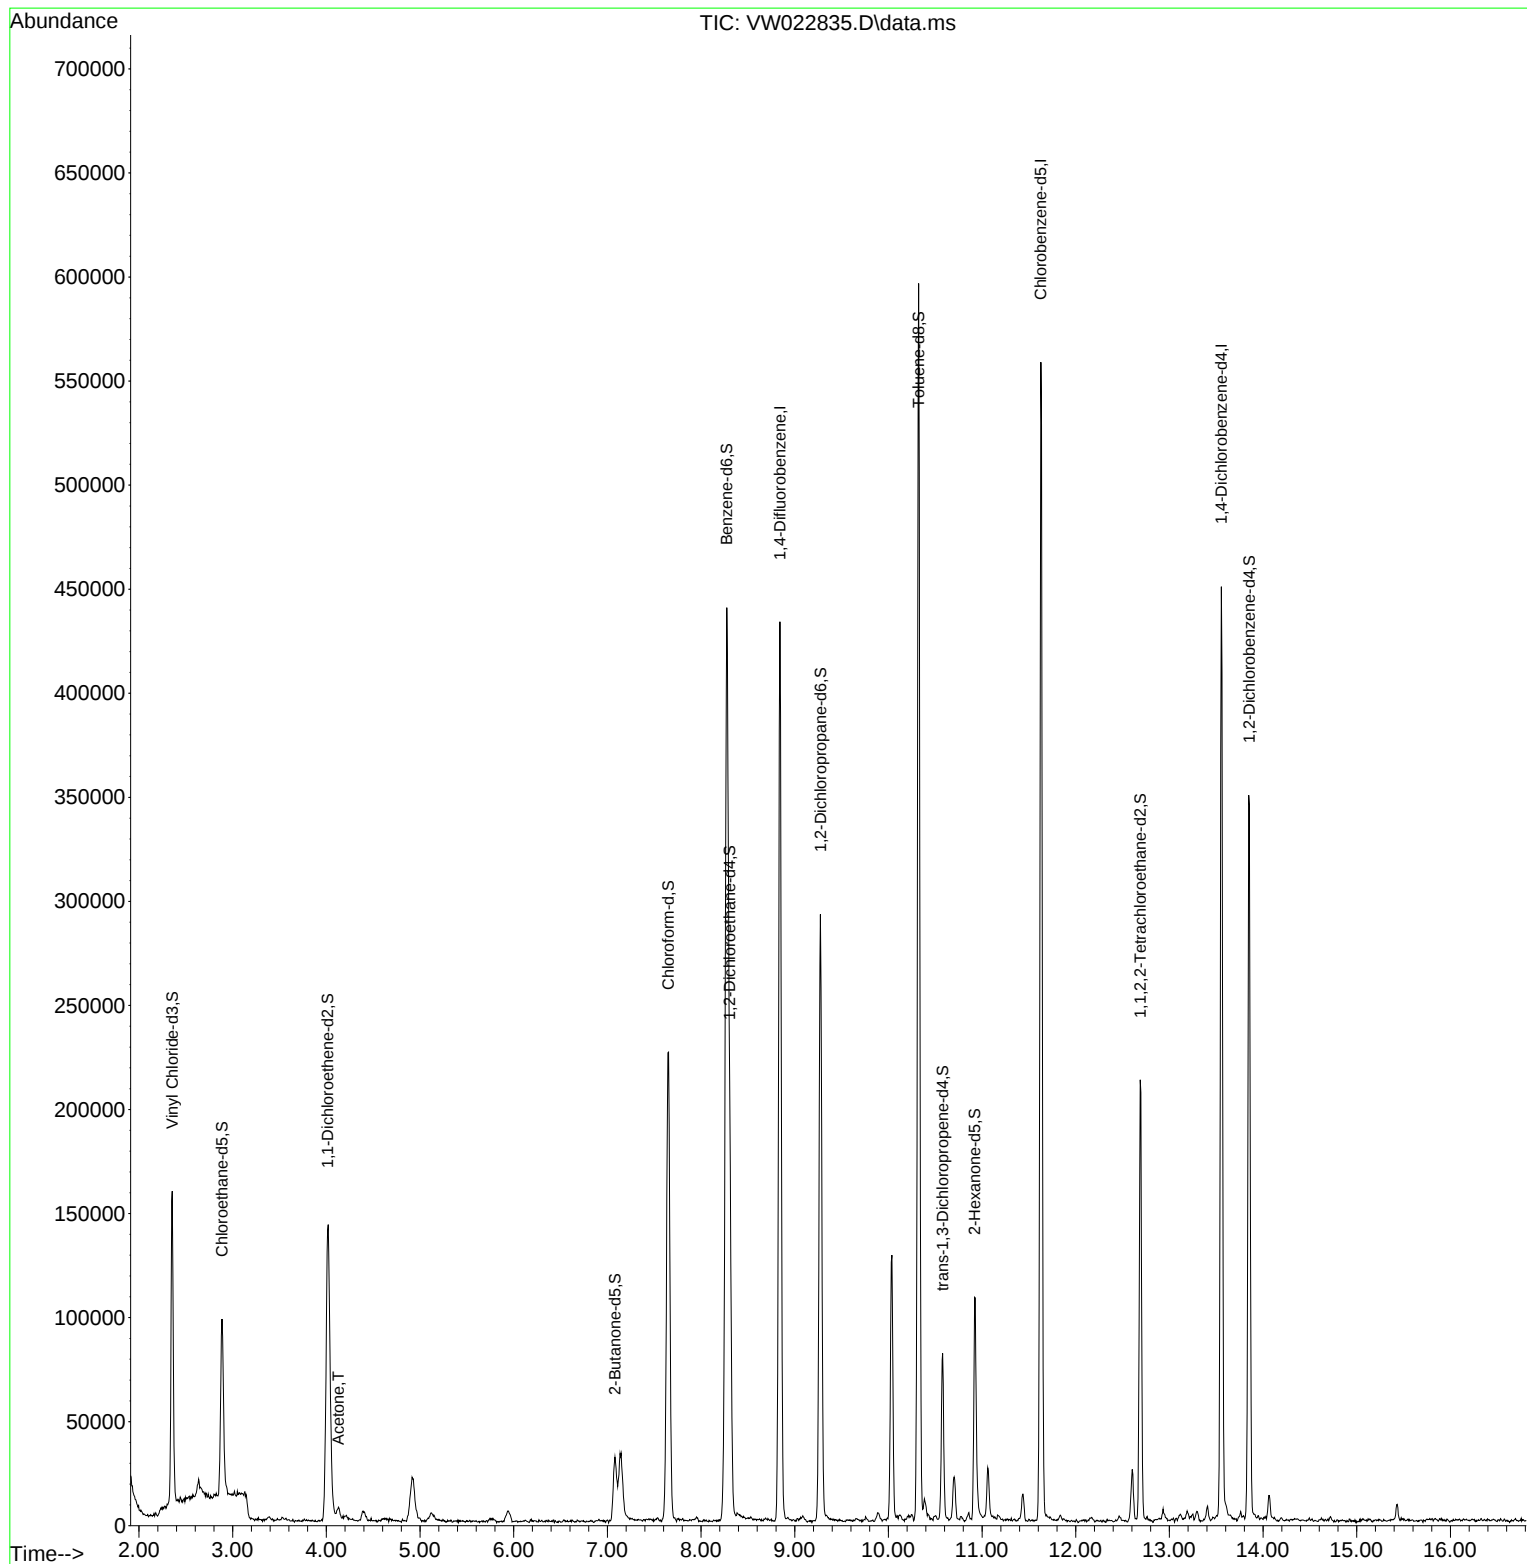

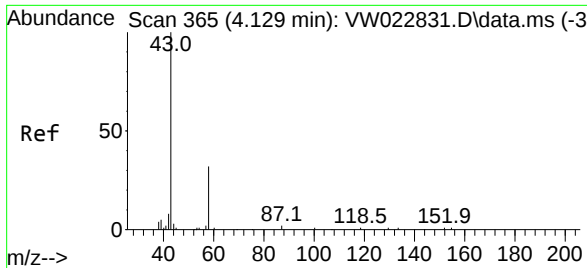

#13
 Acetone
 Concen: 8.862 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW022835.D
 Acq: 05 May 2022 12:24

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBQ7

Tgt Ion: 43 Resp: 9049
 Ion Ratio Lower Upper
 43 100
 58 17.2 0.0 64.0

