

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022839.D
 Acq On : 05 May 2022 14:00
 Operator : SY/VA
 Sample : N2699-11RE
 Misc : 3.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBR4

Quant Time: May 06 01:07:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 01:05:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	330525	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	295361	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	106826	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	143355	21.140	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.560%
7) Chloroethane-d5	2.885	69	105258	23.859	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.440%
11) 1,1-Dichloroethene-d2	4.013	63	132054	15.071	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.280%
21) 2-Butanone-d5	7.080	46	37818	29.332	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.660%
24) Chloroform-d	7.653	84	225843	23.322	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.280%
26) 1,2-Dichloroethane-d4	8.305	65	120207	22.633	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.520%
32) Benzene-d6	8.275	84	418950	24.609	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.440%
36) 1,2-Dichloropropane-d6	9.275	67	123483	25.821	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.280%
41) Toluene-d8	10.323	98	370926	22.555	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.200%
43) trans-1,3-Dichloroprop...	10.579	79	35915	16.311	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.240%
47) 2-Hexanone-d5	10.921	63	27060	29.641	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.280%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	92074	20.657	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.640%
66) 1,2-Dichlorobenzene-d4	13.853	152	83421	22.339	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.360%
Target Compounds					Qvalue	
13) Acetone	4.135	43	3576	3.705	ug/L	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
Data File : VW022839.D
Acq On : 05 May 2022 14:00
Operator : SY/VA
Sample : N2699-11RE
Misc : 3.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGBR4

Quant Time: May 06 01:07:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 06 01:05:05 2022
Response via : Initial Calibration

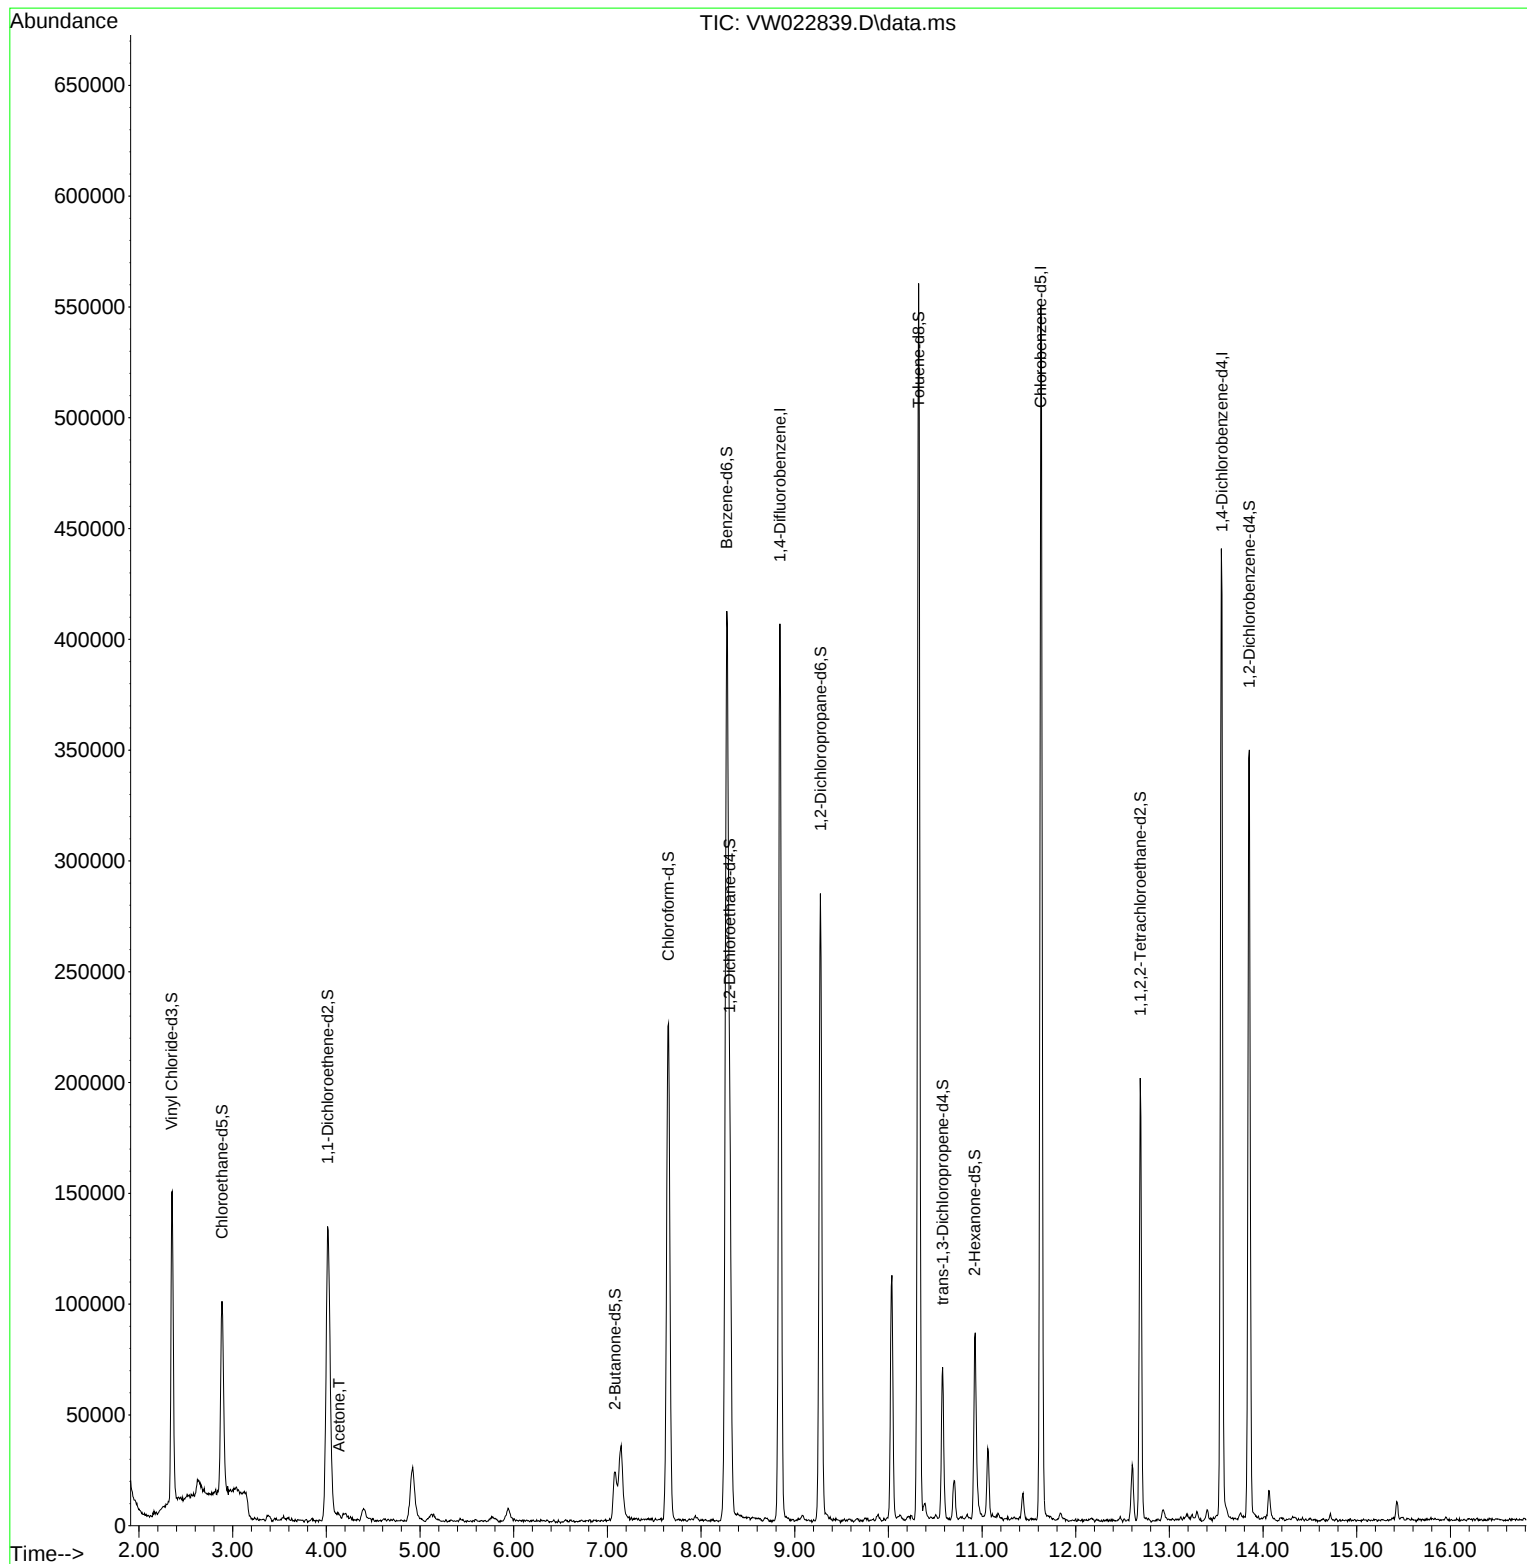

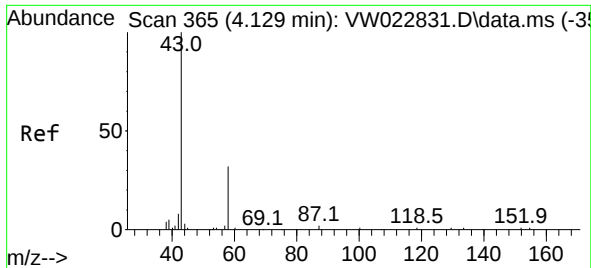

#13
 Acetone
 Concen: 3.705 ug/L
 RT: 4.135 min Scan# 3
 Delta R.T. 0.006 min
 Lab File: VW022839.D
 Acq: 05 May 2022 14:00

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBR4

Tgt Ion: 43 Resp: 3576
 Ion Ratio Lower Upper
 43 100
 58 16.4 0.0 64.0

