

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022847.D
 Acq On : 05 May 2022 17:14
 Operator : SY/VA
 Sample : N2708-02
 Misc : 5.32g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL30

Quant Time: May 06 01:08:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 01:05:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	250806	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	250315	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	118171	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	93517	18.174	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.680%
7) Chloroethane-d5	2.879	69	64699	19.327	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.320%
11) 1,1-Dichloroethene-d2	4.007	63	88141	13.257	ug/L	-0.02
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.040%
21) 2-Butanone-d5	7.074	46	42281	43.217	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.440%
24) Chloroform-d	7.647	84	148747	20.243	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.960%
26) 1,2-Dichloroethane-d4	8.305	65	86031	21.347	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.400%
32) Benzene-d6	8.275	84	283278	19.634	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.520%
36) 1,2-Dichloropropane-d6	9.274	67	84791	20.921	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.680%
41) Toluene-d8	10.323	98	254757	18.279	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.120%
43) trans-1,3-Dichloroprop...	10.579	79	33327	17.859	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.440%
47) 2-Hexanone-d5	10.921	63	32517	42.029	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.060%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	79707	21.100	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.400%
66) 1,2-Dichlorobenzene-d4	13.853	152	85649	20.734	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.920%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	3175	0.574	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
Data File : VW022847.D
Acq On : 05 May 2022 17:14
Operator : SY/VA
Sample : N2708-02
Misc : 5.32g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL30

Quant Time: May 06 01:08:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 06 01:05:05 2022
Response via : Initial Calibration

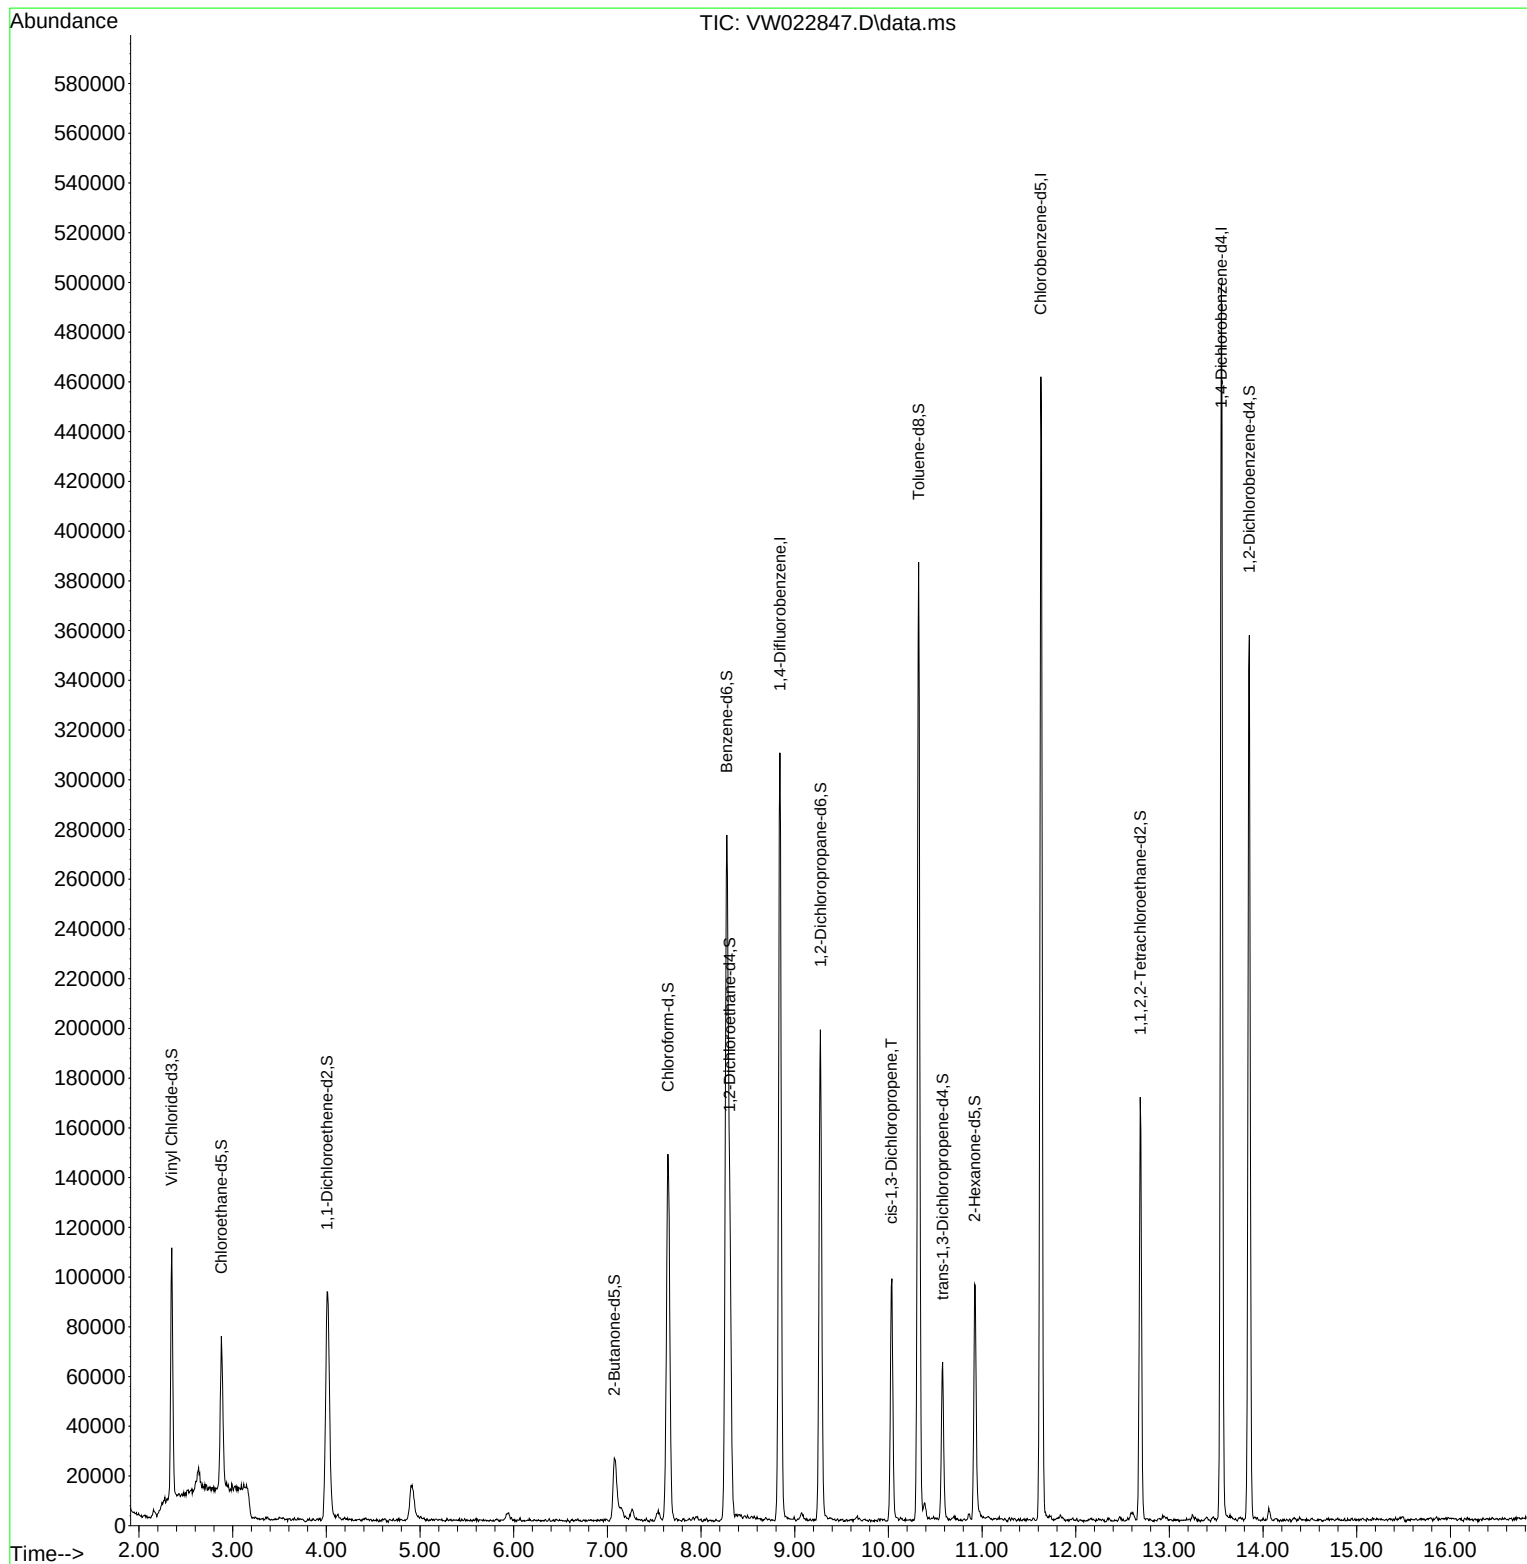

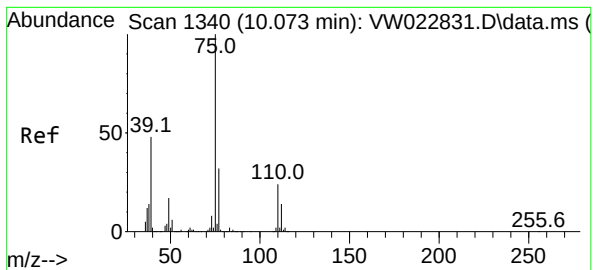

#39
 cis-1,3-Dichloropropene
 Concen: 0.574 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW022847.D
 Acq: 05 May 2022 17:14

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL30

Tgt Ion:	75	Resp:	3175
Ion Ratio	Lower	Upper	
75	100		
77	40.1	22.1	41.1

