

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022856.D
 Acq On : 05 May 2022 21:58
 Operator : SY/VA
 Sample : N2708-13
 Misc : 5.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL39

Quant Time: May 06 02:56:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 02:14:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	322084	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	318210	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	144740	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	125681	19.019	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.080%
7) Chloroethane-d5	2.885	69	98969	23.021	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.080%
11) 1,1-Dichloroethene-d2	4.019	63	118179	13.841	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.360%
21) 2-Butanone-d5	7.080	46	68116	54.215	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.440%
24) Chloroform-d	7.647	84	216127	22.904	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	8.305	65	126652	24.472	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.880%
32) Benzene-d6	8.275	84	405951	22.133	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.520%
36) 1,2-Dichloropropane-d6	9.275	67	123748	24.019	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.080%
41) Toluene-d8	10.323	98	373397	21.075	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.280%
43) trans-1,3-Dichloroprop...	10.579	79	50061	21.103	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.400%
47) 2-Hexanone-d5	10.927	63	54391	55.301	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.600%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	120461	25.085	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	122528	24.217	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.880%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4531	0.644	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
Data File : VW022856.D
Acq On : 05 May 2022 21:58
Operator : SY/VA
Sample : N2708-13
Misc : 5.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL39

Quant Time: May 06 02:56:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 06 02:14:27 2022
Response via : Initial Calibration

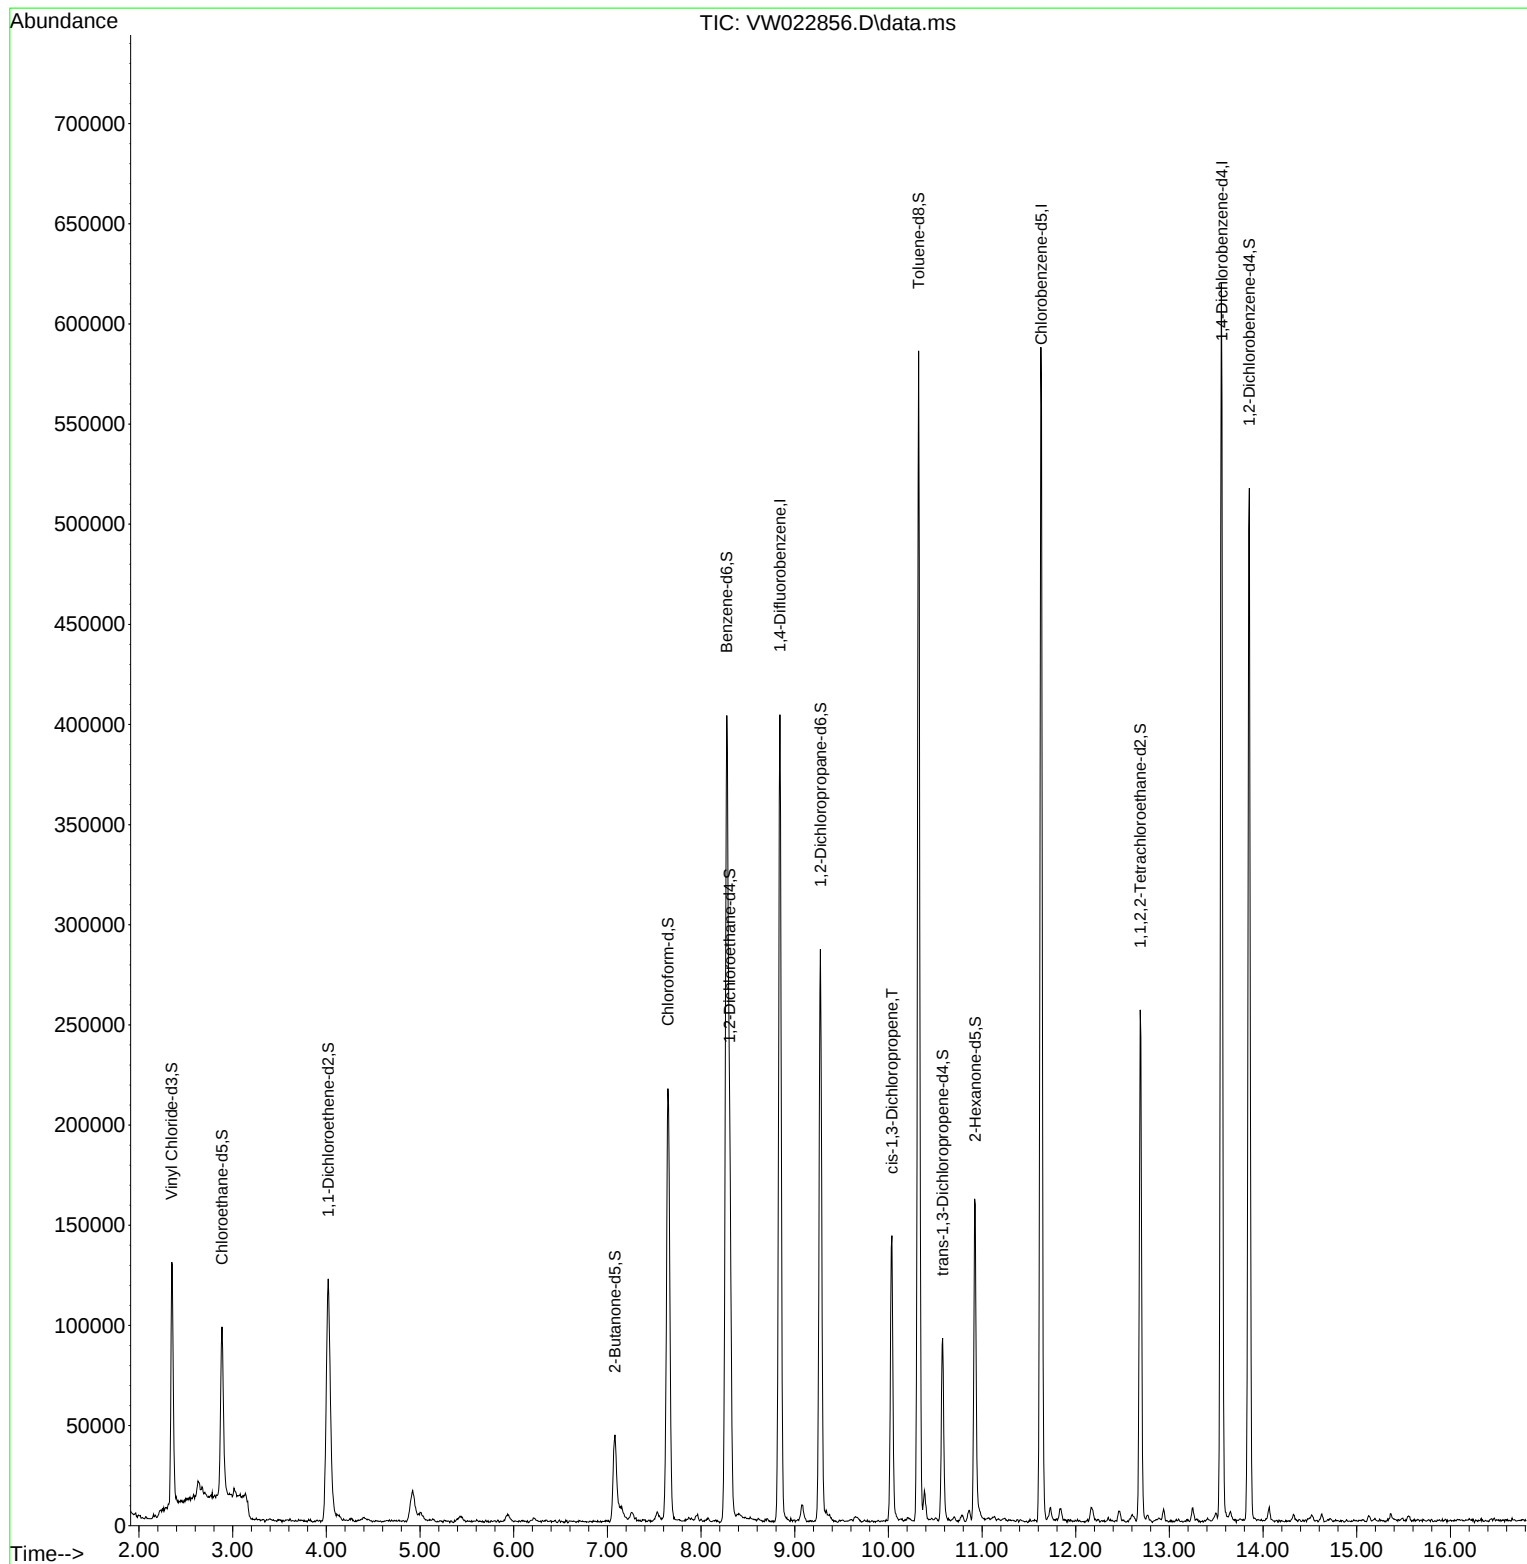

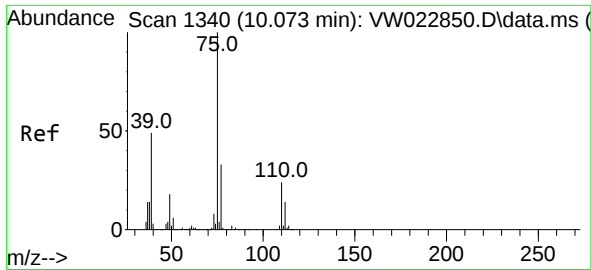

#39
 cis-1,3-Dichloropropene
 Concen: 0.644 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022856.D
 Acq: 05 May 2022 21:58

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL39

Tgt Ion: 75 Resp: 4531
 Ion Ratio Lower Upper
 75 100
 77 34.5 22.1 41.1

