

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022860.D
 Acq On : 05 May 2022 23:34
 Operator : SY/VA
 Sample : N2708-17
 Misc : 4.87g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL43

Quant Time: May 06 02:57:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 02:14:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	333873	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	322648	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	151684	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	119919	17.507	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.040%
7) Chloroethane-d5	2.885	69	88611	19.884	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.520%
11) 1,1-Dichloroethene-d2	4.013	63	112945	12.761	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.040%
21) 2-Butanone-d5	7.080	46	63464	48.729	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.460%
24) Chloroform-d	7.647	84	207881	21.252	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.000%
26) 1,2-Dichloroethane-d4	8.195	65	72	0.013	ug/L	-0.11
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.275	84	399243	21.468	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.880%
36) 1,2-Dichloropropane-d6	9.274	67	120789	23.122	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.480%
41) Toluene-d8	10.323	98	365583	20.350	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.400%
43) trans-1,3-Dichloroprop...	10.579	79	48551	20.185	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.720%
47) 2-Hexanone-d5	10.920	63	50757	50.897	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.800%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	115098	23.638	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	119569	22.550	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.200%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4441	0.623	ug/L	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
Data File : VW022860.D
Acq On : 05 May 2022 23:34
Operator : SY/VA
Sample : N2708-17
Misc : 4.87g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL43

Quant Time: May 06 02:57:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 06 02:14:27 2022
Response via : Initial Calibration

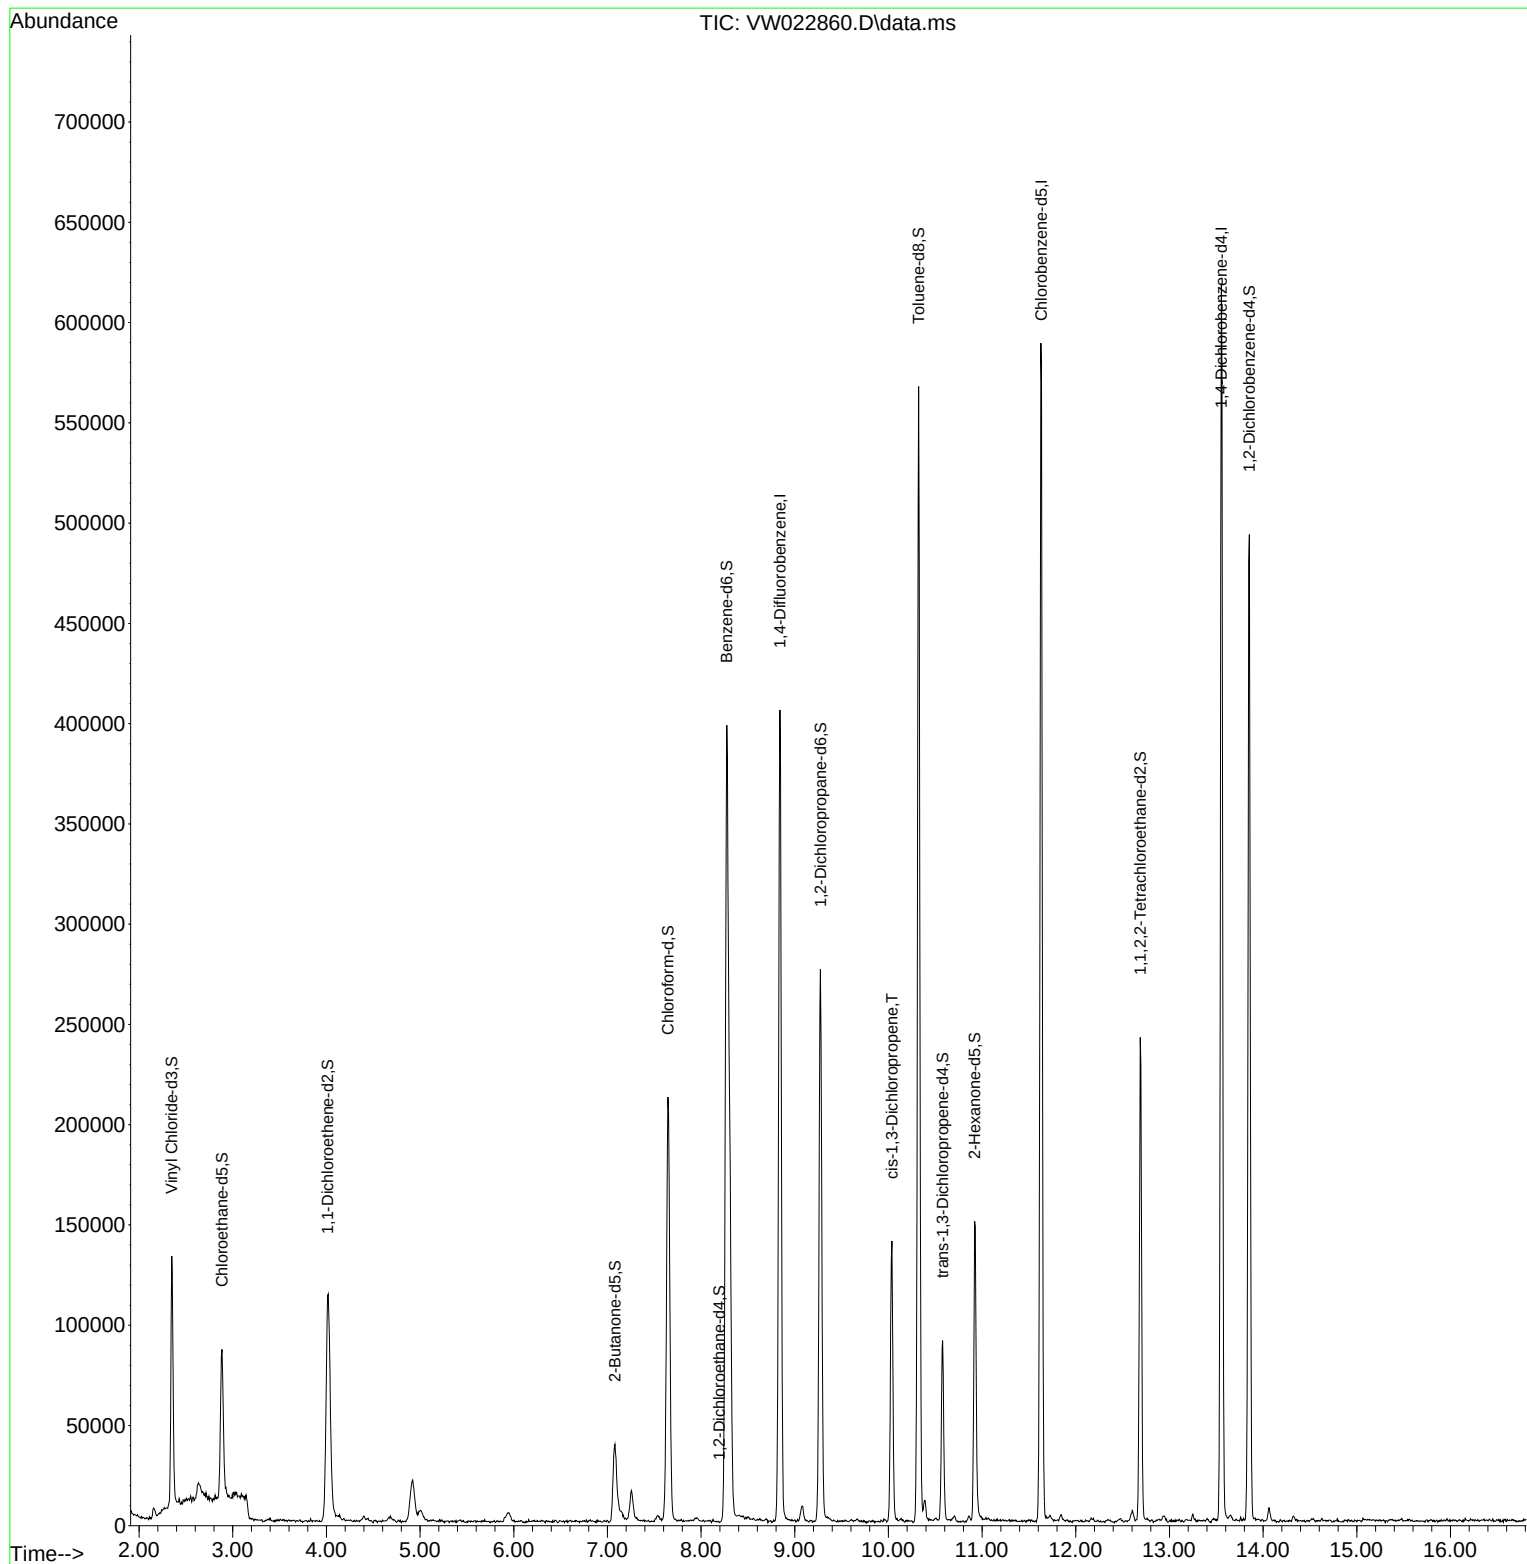

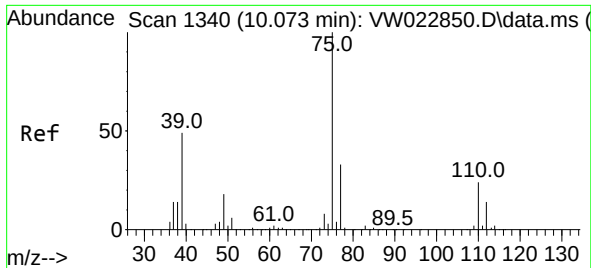

#39
 cis-1,3-Dichloropropene
 Concen: 0.623 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022860.D
 Acq: 05 May 2022 23:34

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL43

Tgt Ion: 75 Resp: 4441
 Ion Ratio Lower Upper
 75 100
 77 44.6 22.1 41.1#

