




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022853.D
 Acq On : 05 May 2022 20:45
 Operator : SY/VA
 Sample : N2708-10
 Misc : 5.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL36

Manual IntegrationsAPPROVED

Quant Time: May 06 02:56:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 02:14:27 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

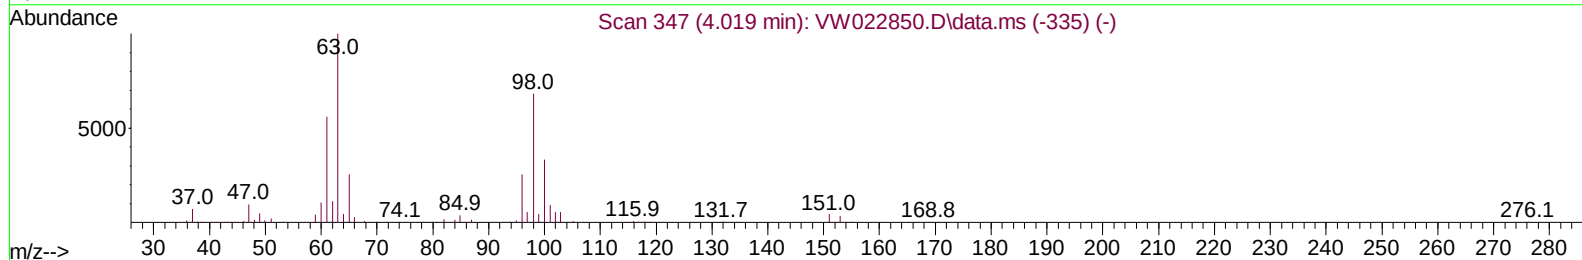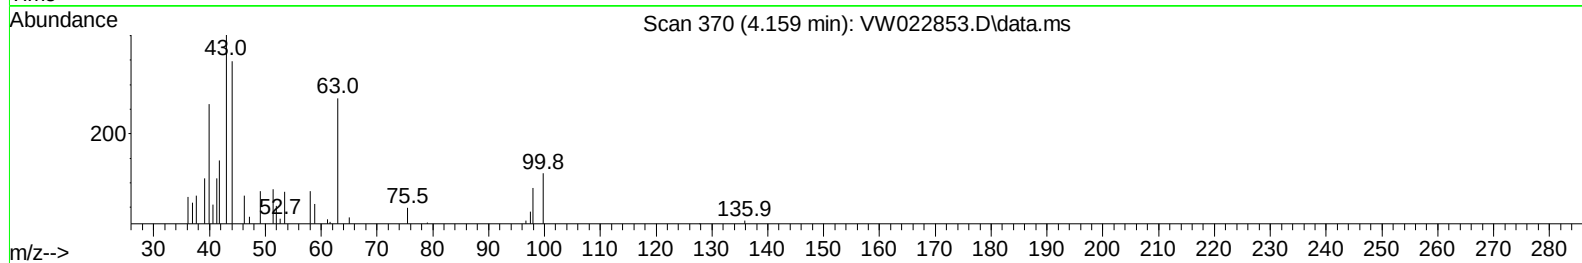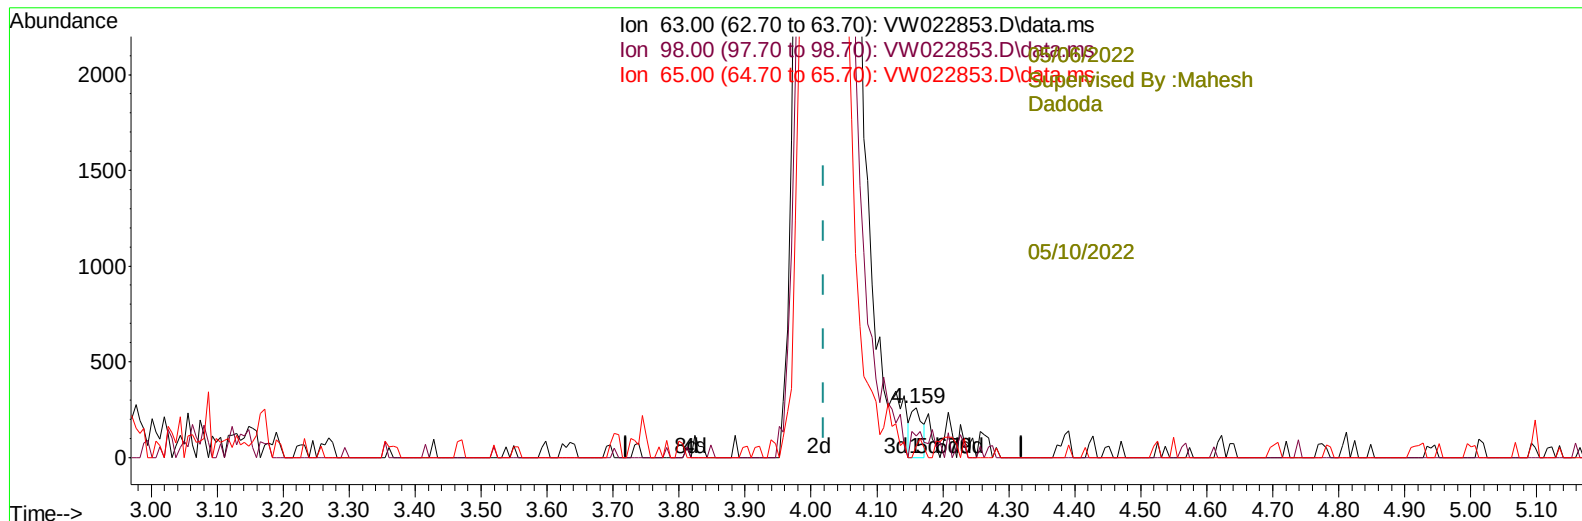

TIC: VW022853.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.159min (+ 0.140) 0.03 ug/L

response 313

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	62.30
65.00	23.30	25.24
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022853.D
 Acq On : 05 May 2022 20:45
 Operator : SY/VA
 Sample : N2708-10
 Misc : 5.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL36

Manual IntegrationsAPPROVED

Quant Time: May 06 02:56:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 02:14:27 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

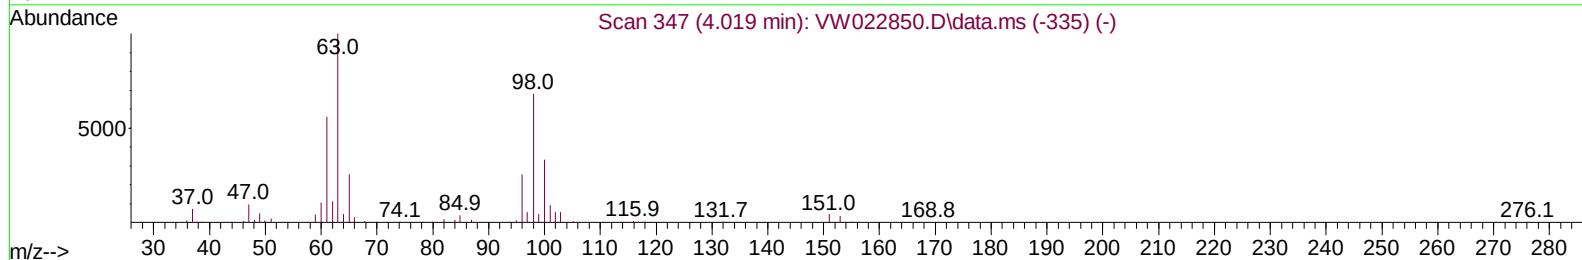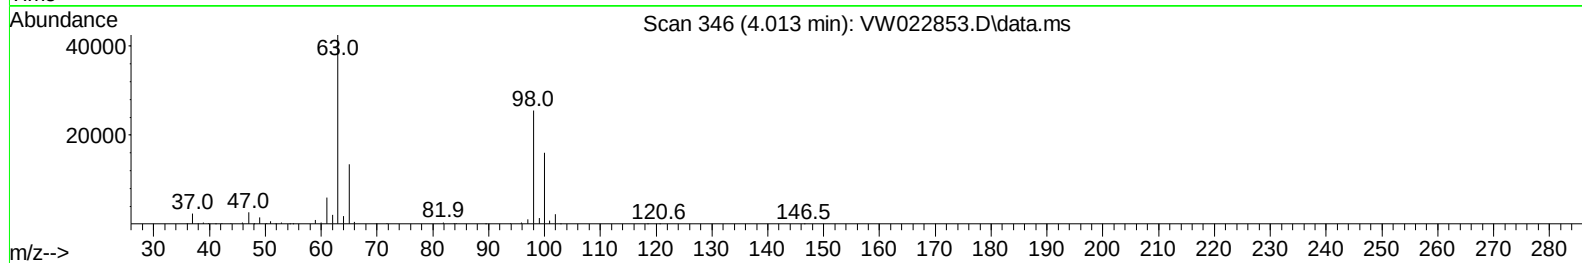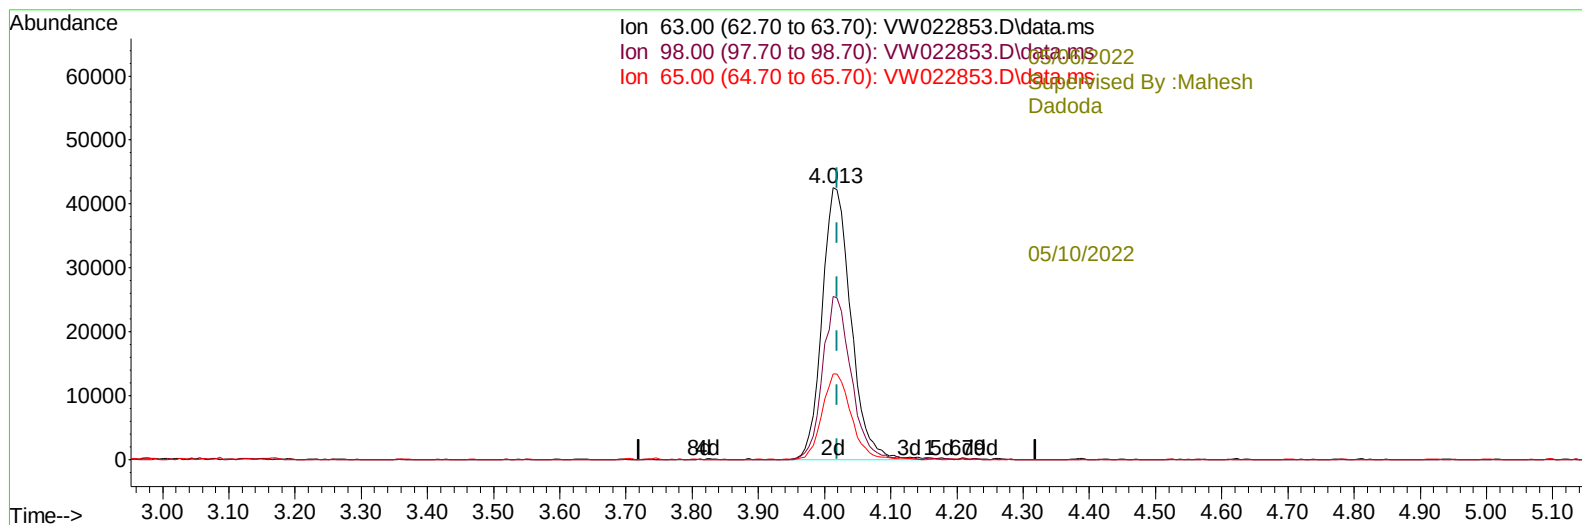

TIC: VW022853.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 13.71 ug/L m

response 128146

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.15#
65.00	23.30	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022853.D
 Acq On : 05 May 2022 20:45
 Operator : SY/VA
 Sample : N2708-10
 Misc : 5.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL36

Manual IntegrationsAPPROVED

Quant Time: May 06 02:56:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 02:14:27 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----05/06/2022-----							
Supervised By :Mahesh							
Padoda							
Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		352469	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117		335130	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		168160	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		138929	19.212	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.840%	
7) Chloroethane-d5	2.891	69		103200	21.936	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.760%	
11) 1,1-Dichloroethene-d2	4.013	63		128146m	13.715	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.840%	
21) 2-Butanone-d5	7.080	46		67403	49.023	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.040%	
24) Chloroform-d	7.646	84		231641	22.432	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.720%	
26) 1,2-Dichloroethane-d4	8.305	65		133424	23.558	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.240%	
32) Benzene-d6	8.274	84		438697	22.711	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.840%	
36) 1,2-Dichloropropane-d6	9.274	67		132792	24.473	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.880%	
41) Toluene-d8	10.323	98		403936	21.647	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.600%	
43) trans-1,3-Dichloroprop...	10.579	79		53246	21.312	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.240%	
47) 2-Hexanone-d5	10.926	63		56505	54.550	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.100%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		125060	24.728	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.920%	
66) 1,2-Dichlorobenzene-d4	13.853	152		141928	24.144	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.560%	
Target Compounds							
46) Tetrachloroethene	10.859	164		3379	0.828	ug/L #	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
Data File : VW022853.D
Acq On : 05 May 2022 20:45
Operator : SY/VA
Sample : N2708-10
Misc : 5.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL36

Manual IntegrationsAPPROVED

Quant Time: May 06 02:56:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 06 02:14:27 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

