

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022846.D
 Acq On : 05 May 2022 16:49
 Operator : SY/VA
 Sample : N2708-08
 Misc : 4.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL34

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/06/2022
 Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 06 01:08:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 01:05:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	354418	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	315395	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	127672	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	143127	19.684	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.720%		
7) Chloroethane-d5	2.885	69	110872	23.437	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.760%		
11) 1,1-Dichloroethene-d2	4.013	63	129822	13.817	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	55.280%		
21) 2-Butanone-d5	7.080	46	60110	43.478	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.960%		
24) Chloroform-d	7.647	84	226998	21.861	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.440%		
26) 1,2-Dichloroethane-d4	8.305	65	129240m	22.694	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.760%		
32) Benzene-d6	8.275	84	427421	23.512	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.040%		
36) 1,2-Dichloropropane-d6	9.275	67	129879	25.434	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.720%		
41) Toluene-d8	10.323	98	379049	21.585	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.320%		
43) trans-1,3-Dichloroprop...	10.579	79	46505	19.779	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.120%		
47) 2-Hexanone-d5	10.921	63	47628	48.857	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	97.720%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	113709	23.890	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	95.560%		
66) 1,2-Dichlorobenzene-d4	13.847	152	100200	22.451	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.800%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	3179	3.071	ug/L	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
Data File : VW022846.D
Acq On : 05 May 2022 16:49
Operator : SY/VA
Sample : N2708-08
Misc : 4.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EXL34

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/06/2022
Supervised By :Mahesh Dadoda 05/10/2022


Quant Time: May 06 01:08:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 06 01:05:05 2022
Response via : Initial Calibration

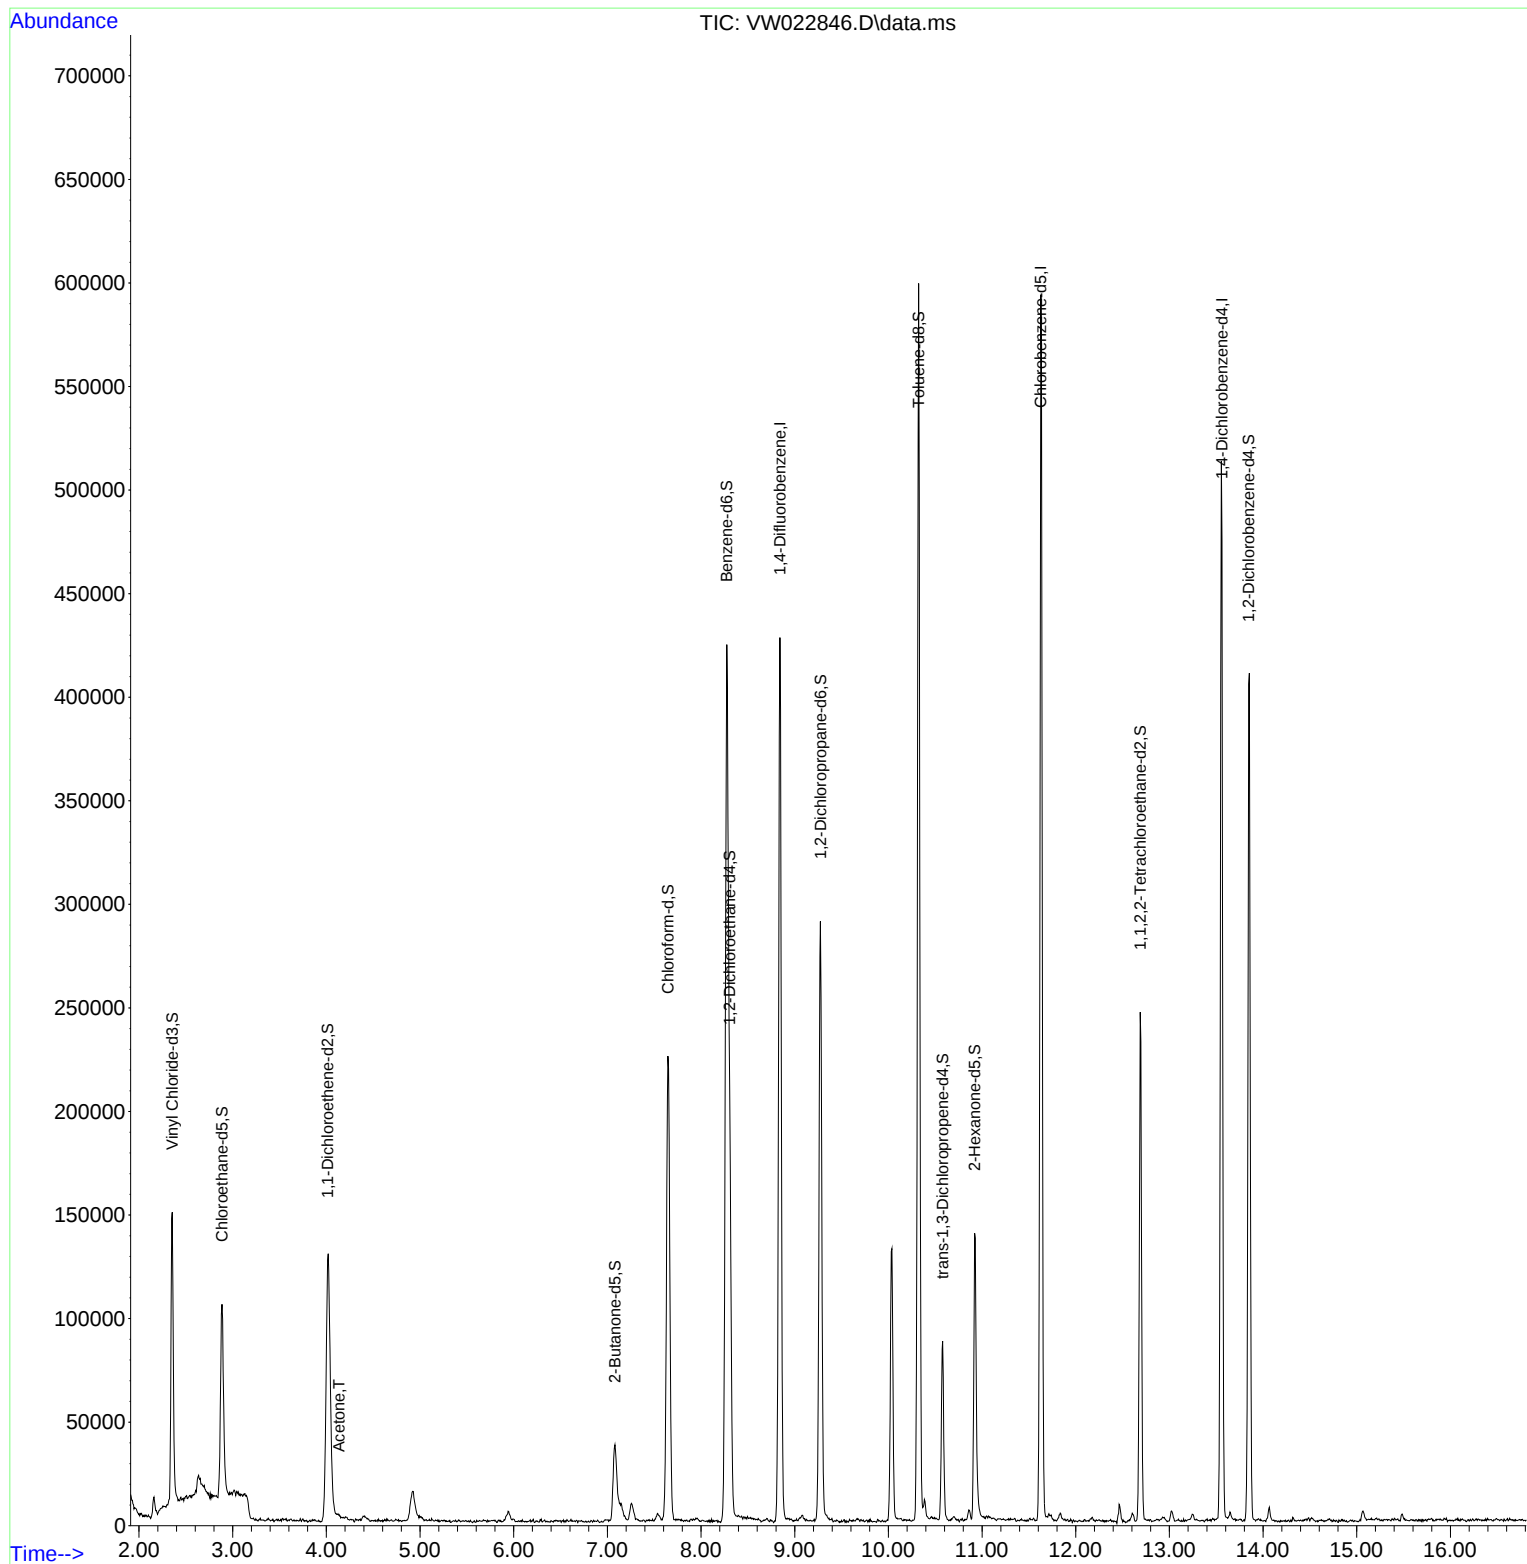

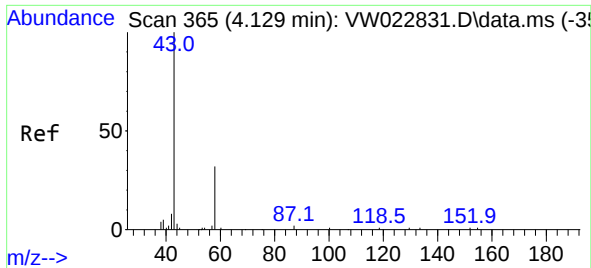

#13
Acetone
Concen: 3.071 ug/L
RT: 4.135 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW022846.D
Acq: 05 May 2022 16:49

Instrument :
MSVOA_W
ClientSampleId :
EXL34

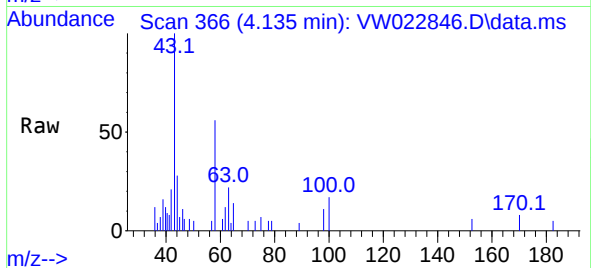

Tgt Ion: 43 Resp: 3179
Ion Ratio Lower Upper
43 100
58 14.7 0.0 64.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/06/2022
Supervised By :Mahesh Dadoda 05/10/2022

