

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
 Data File : VW022873.D
 Acq On : 06 May 2022 04:48
 Operator : SY/VA
 Sample : N2709-10
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL58

Quant Time: May 06 05:11:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 06 02:14:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	327973	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	315468	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	143238	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	123525	18.358	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.440%
7) Chloroethane-d5	2.885	69	96054	21.942	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.760%
11) 1,1-Dichloroethene-d2	4.019	63	119253	13.716	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.880%
21) 2-Butanone-d5	7.080	46	59527	46.528	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.060%
24) Chloroform-d	7.647	84	213982	22.269	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.080%
26) 1,2-Dichloroethane-d4	8.305	65	122277	23.202	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	8.275	84	407003	22.383	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.520%
36) 1,2-Dichloropropane-d6	9.275	67	122892	24.060	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.240%
41) Toluene-d8	10.323	98	367685	20.933	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.720%
43) trans-1,3-Dichloroprop...	10.573	79	44915	19.098	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.400%
47) 2-Hexanone-d5	10.921	63	47686	48.906	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.820%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	108288	22.746	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.000%
66) 1,2-Dichlorobenzene-d4	13.847	152	111700	22.308	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.240%
Target Compounds					Qvalue	
25) Chloroform	7.677	83	4682	0.529	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050522\
Data File : VW022873.D
Acq On : 06 May 2022 04:48
Operator : SY/VA
Sample : N2709-10
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL58

Quant Time: May 06 05:11:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 06 02:14:27 2022
Response via : Initial Calibration

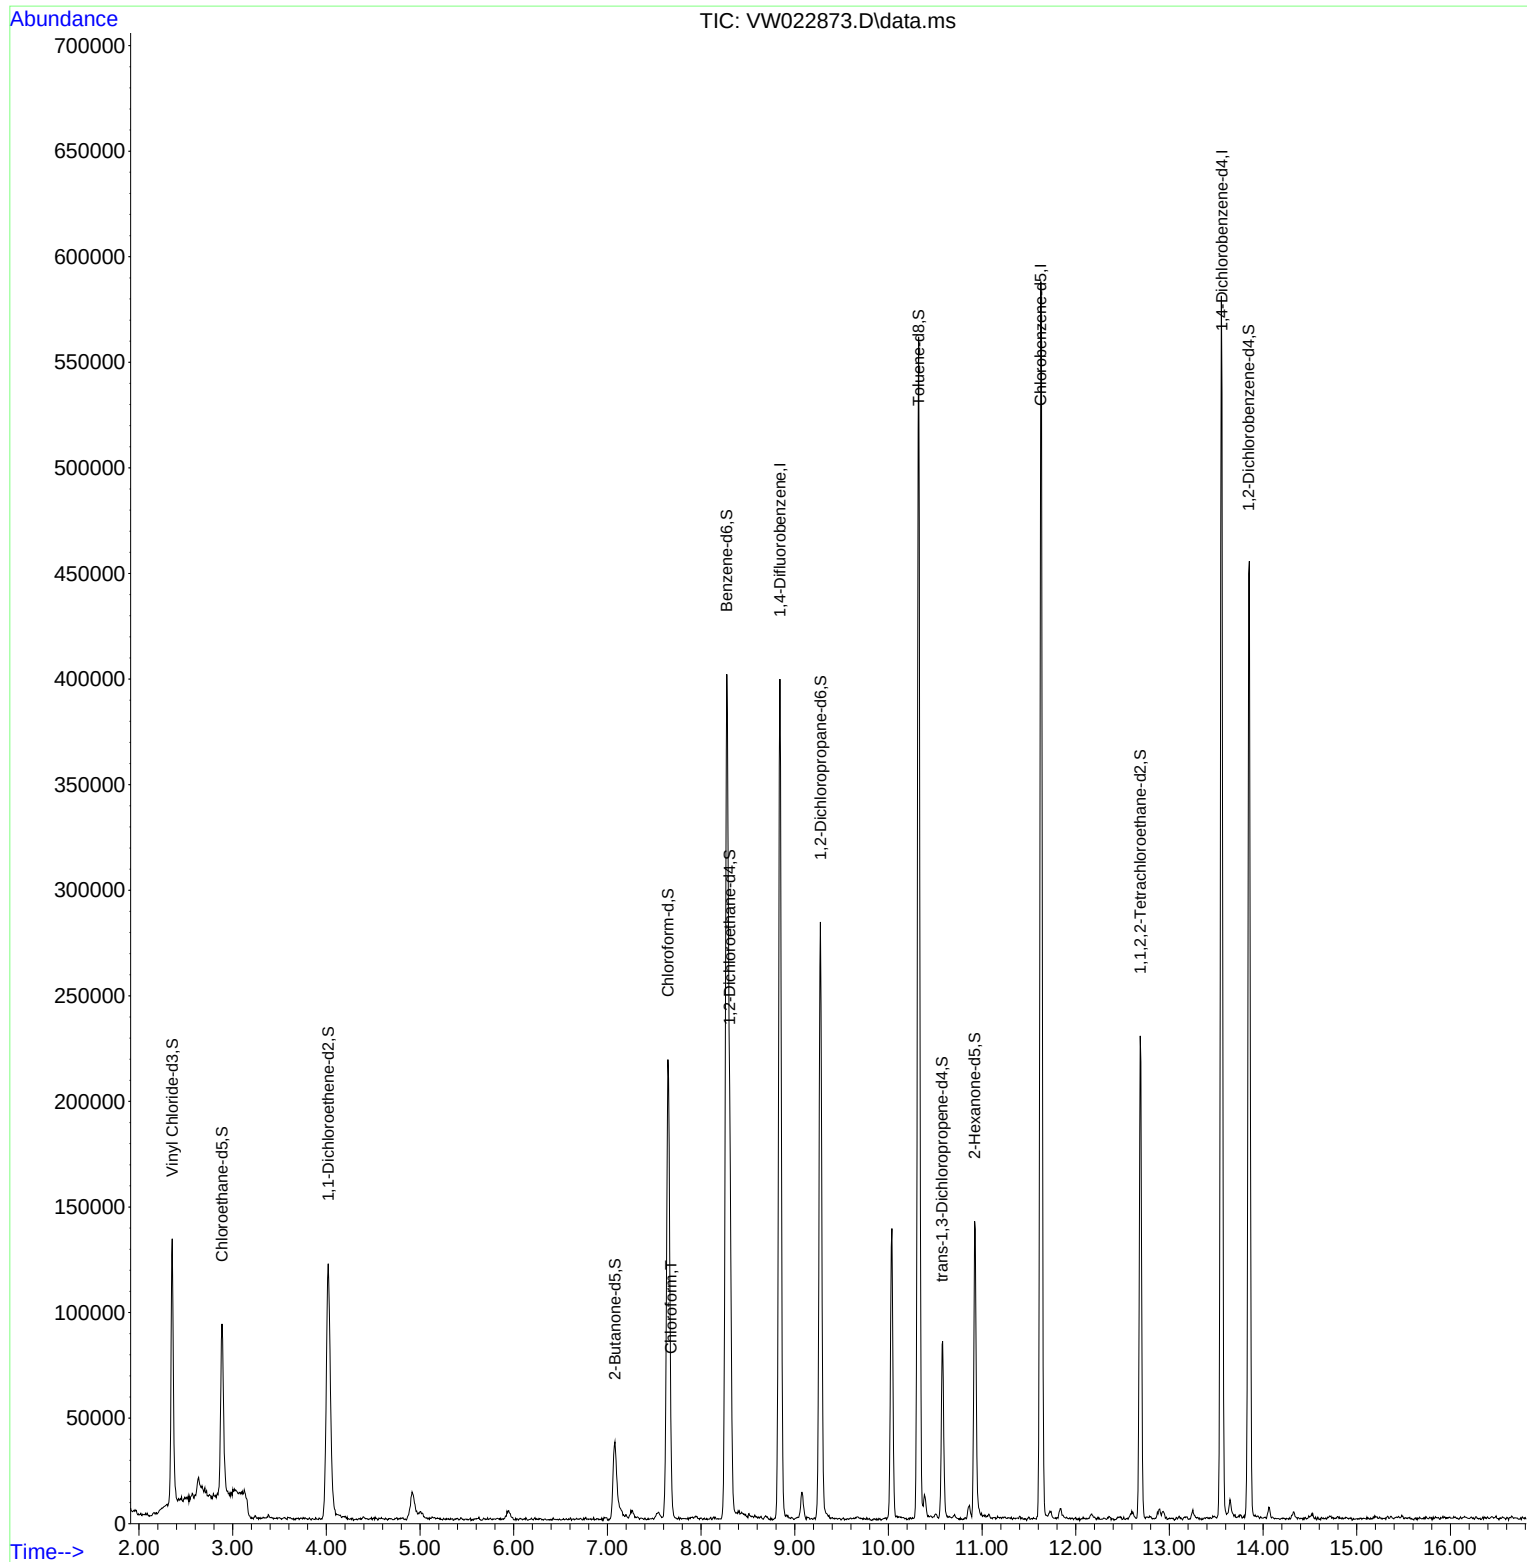

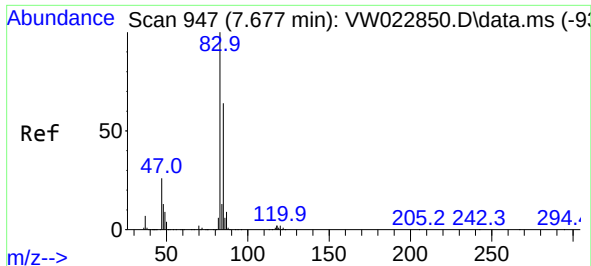

#25
Chloroform
Concen: 0.529 ug/L
RT: 7.677 min Scan# 94
Delta R.T. 0.000 min
Lab File: VW022873.D
Acq: 06 May 2022 04:48

Instrument :
MSVOA_W
ClientSampleId :
EXL58

Tgt Ion: 83 Resp: 4682
Ion Ratio Lower Upper
83 100
85 72.4 46.6 86.6

