

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022880.D
 Acq On : 06 May 2022 11:15
 Operator : SY/VA
 Sample : N2632-03
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 07 00:03:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 00:02:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	297607	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	293896	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	148692	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	127031	20.805	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.200%
7) Chloroethane-d5	2.885	69	87691	22.075	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.320%
11) 1,1-Dichloroethene-d2	4.019	63	124189	15.741	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.960%
21) 2-Butanone-d5	7.074	46	58488	50.381	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.760%
24) Chloroform-d	7.653	84	206630	23.698	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	8.305	65	118603	24.801	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	8.275	84	398340	23.515	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.040%
36) 1,2-Dichloropropane-d6	9.274	67	117071	24.603	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.400%
41) Toluene-d8	10.323	98	369898	22.604	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.400%
43) trans-1,3-Dichloroprop...	10.579	79	47390	21.629	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.520%
47) 2-Hexanone-d5	10.920	63	45810	50.430	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.860%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	111379	25.112	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	127368	24.504	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.000%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.043	75	4641	0.714	ug/L	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022880.D
Acq On : 06 May 2022 11:15
Operator : SY/VA
Sample : N2632-03
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 07 00:03:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 00:02:41 2022
Response via : Initial Calibration

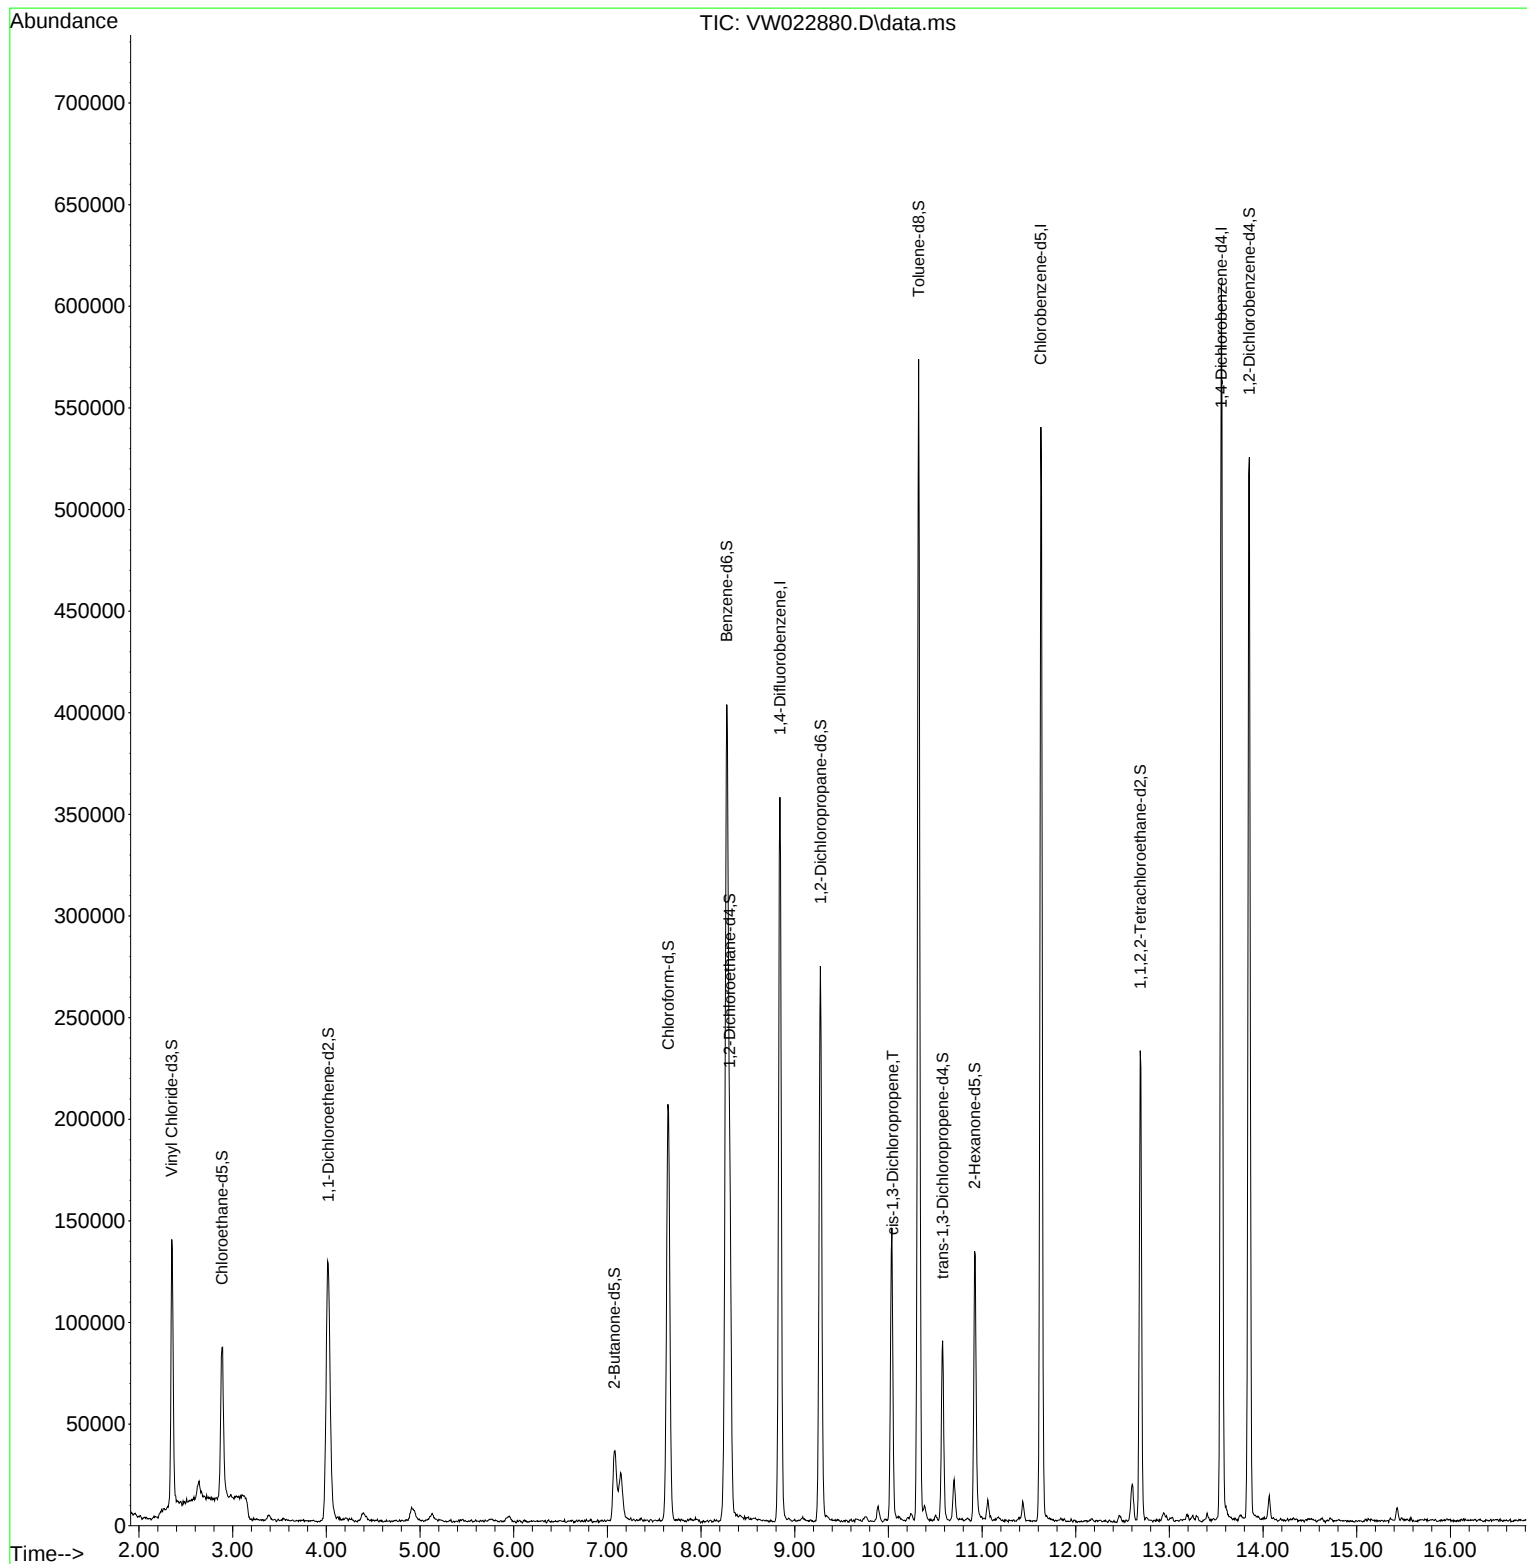

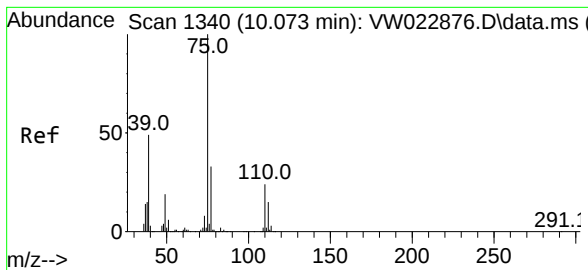

#39
 cis-1,3-Dichloropropene
 Concen: 0.714 ug/L
 RT: 10.043 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW022880.D
 Acq: 06 May 2022 11:15

Instrument :
 MSVOA_W
 ClientSampleId :

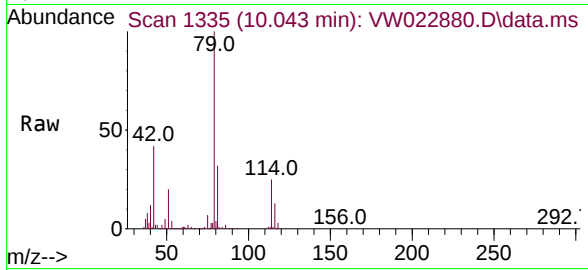

Tgt Ion: 75 Resp: 4641
 Ion Ratio Lower Upper
 75 100
 77 41.6 22.1 41.1#

