

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022881.D
 Acq On : 06 May 2022 11:39
 Operator : SY/VA
 Sample : N2699-13
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 07 00:04:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 00:02:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	314935	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	302272	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	153173	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	130091	20.134	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.520%
7) Chloroethane-d5	2.886	69	93641	22.276	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.120%
11) 1,1-Dichloroethene-d2	4.013	63	127106	15.224	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.880%
21) 2-Butanone-d5	7.074	46	58432	47.563	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.120%
24) Chloroform-d	7.647	84	206108	22.338	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.360%
26) 1,2-Dichloroethane-d4	8.305	65	117067	23.133	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.520%
32) Benzene-d6	8.275	84	402142	23.081	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.320%
36) 1,2-Dichloropropane-d6	9.275	67	117515	24.012	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.040%
41) Toluene-d8	10.323	98	375112	22.288	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.160%
43) trans-1,3-Dichloroprop...	10.579	79	46624	20.690	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.760%
47) 2-Hexanone-d5	10.927	63	43857	46.942	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.880%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	106254	23.293	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	124455	23.243	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.960%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4479	0.670	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022881.D
Acq On : 06 May 2022 11:39
Operator : SY/VA
Sample : N2699-13
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 07 00:04:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 00:02:41 2022
Response via : Initial Calibration

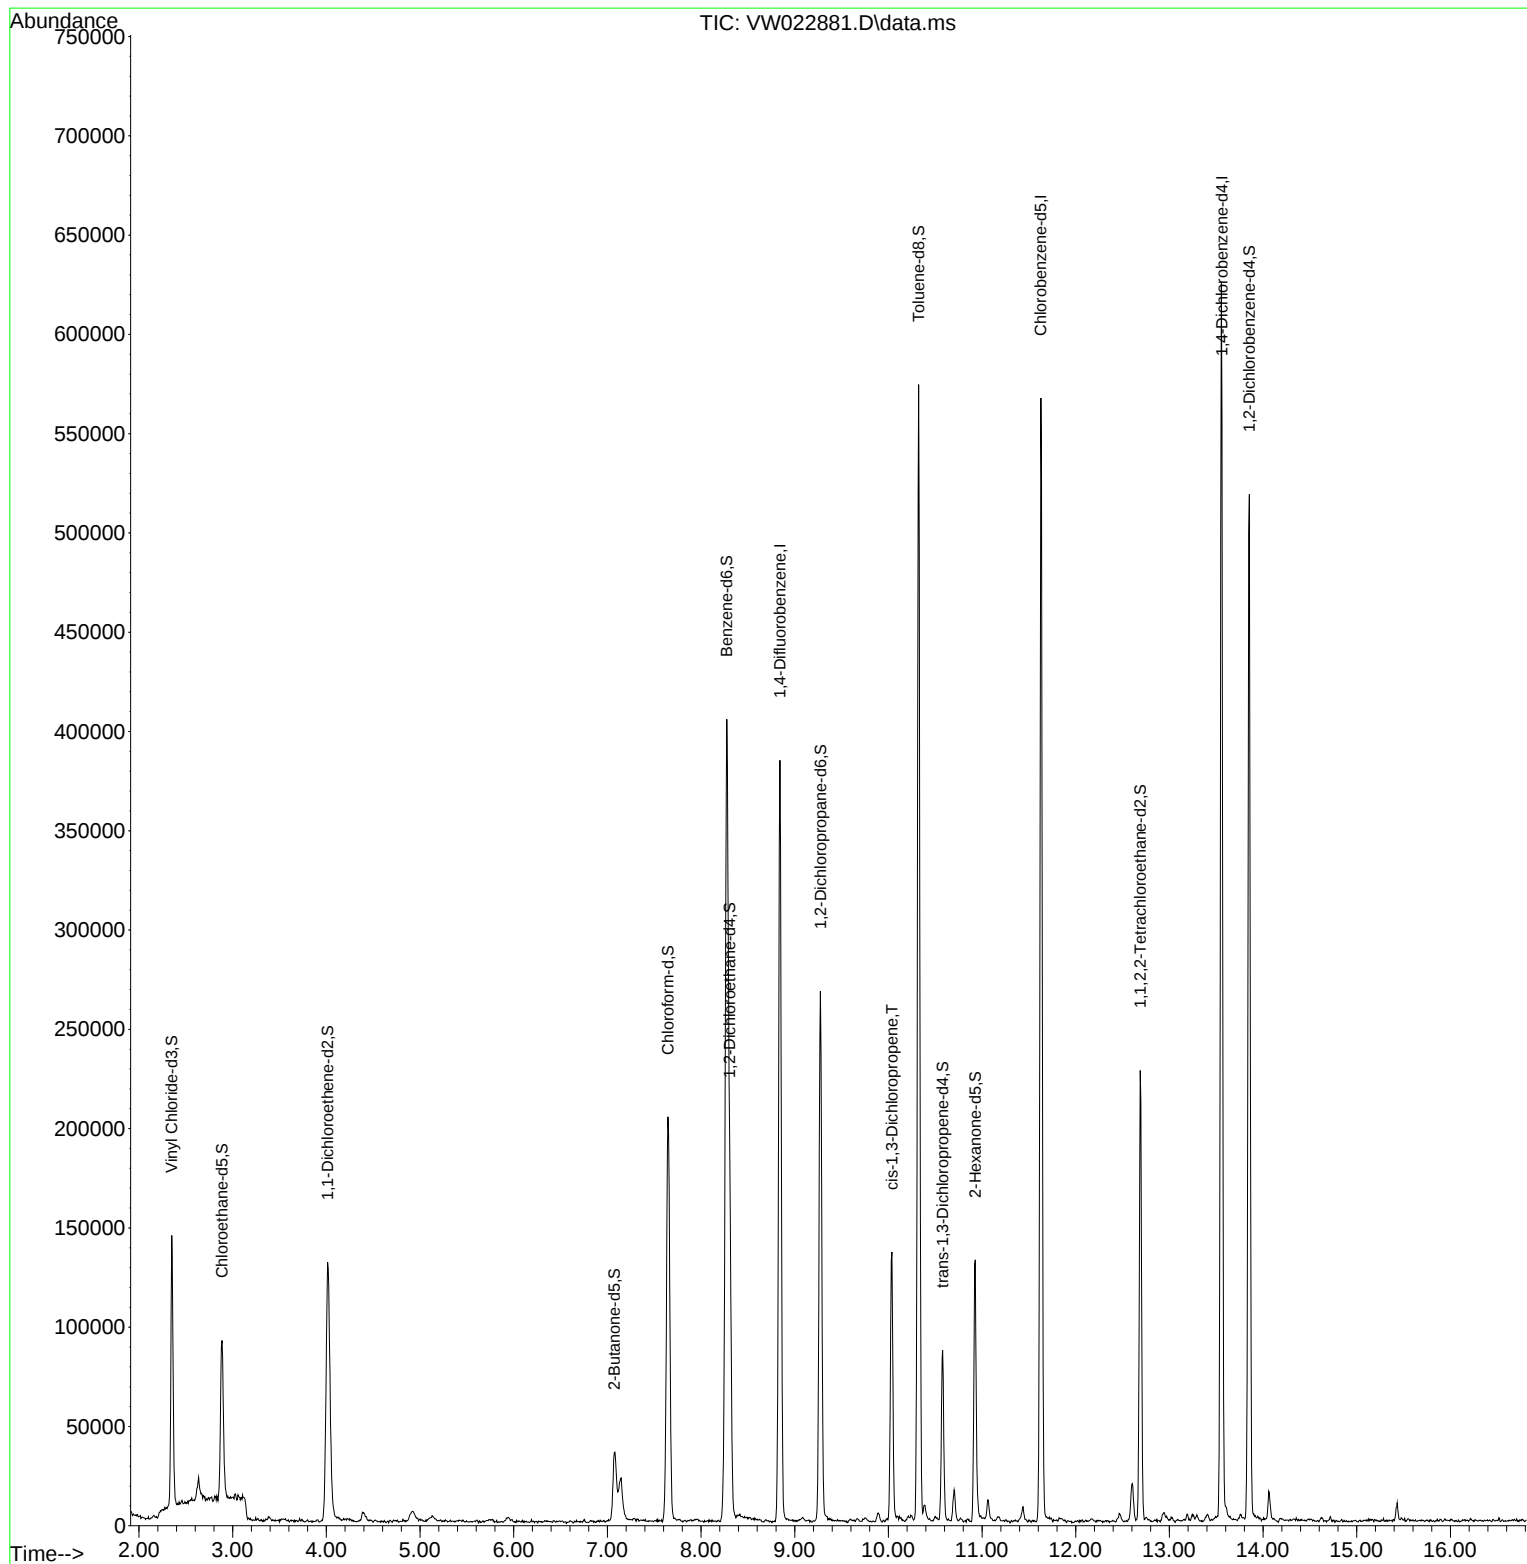

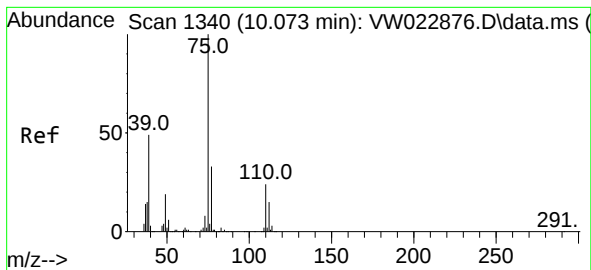

#39
 cis-1,3-Dichloropropene
 Concen: 0.670 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022881.D
 Acq: 06 May 2022 11:39

Instrument :
 MSVOA_W
 ClientSampleId :

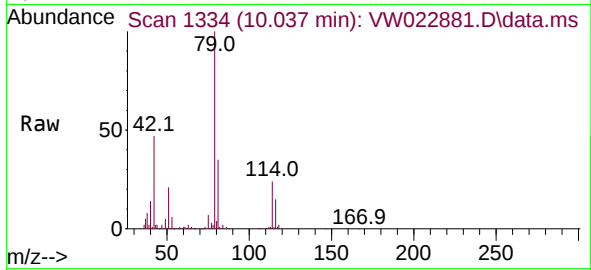

Tgt Ion: 75 Resp: 4479
 Ion Ratio Lower Upper
 75 100
 77 37.6 22.1 41.1

