

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022894.D
 Acq On : 06 May 2022 16:55
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 07 00:06:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 00:02:41 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	304878	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	299242	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	149652	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	124703	19.936	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.760%
7) Chloroethane-d5	2.885	69	94448	23.209	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.840%
11) 1,1-Dichloroethene-d2	4.019	63	121979	15.092	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.360%
21) 2-Butanone-d5	7.074	46	57105	48.017	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.040%
24) Chloroform-d	7.647	84	201437	22.552	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.200%
26) 1,2-Dichloroethane-d4	8.305	65	115903	23.659	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.640%
32) Benzene-d6	8.275	84	384553	22.295	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	9.274	67	114530	23.639	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.560%
41) Toluene-d8	10.323	98	362941	21.783	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.120%
43) trans-1,3-Dichloroprop...	10.579	79	45391	20.347	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.400%
47) 2-Hexanone-d5	10.920	63	44926	48.573	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.140%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	105197	23.295	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.160%
66) 1,2-Dichlorobenzene-d4	13.847	152	121591	23.243	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.960%
Target Compounds						
39) cis-1,3-Dichloropropene	10.036	75	3897	0.589	ug/L	Qvalue # 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022894.D
Acq On : 06 May 2022 16:55
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 07 00:06:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 00:02:41 2022
Response via : Initial Calibration

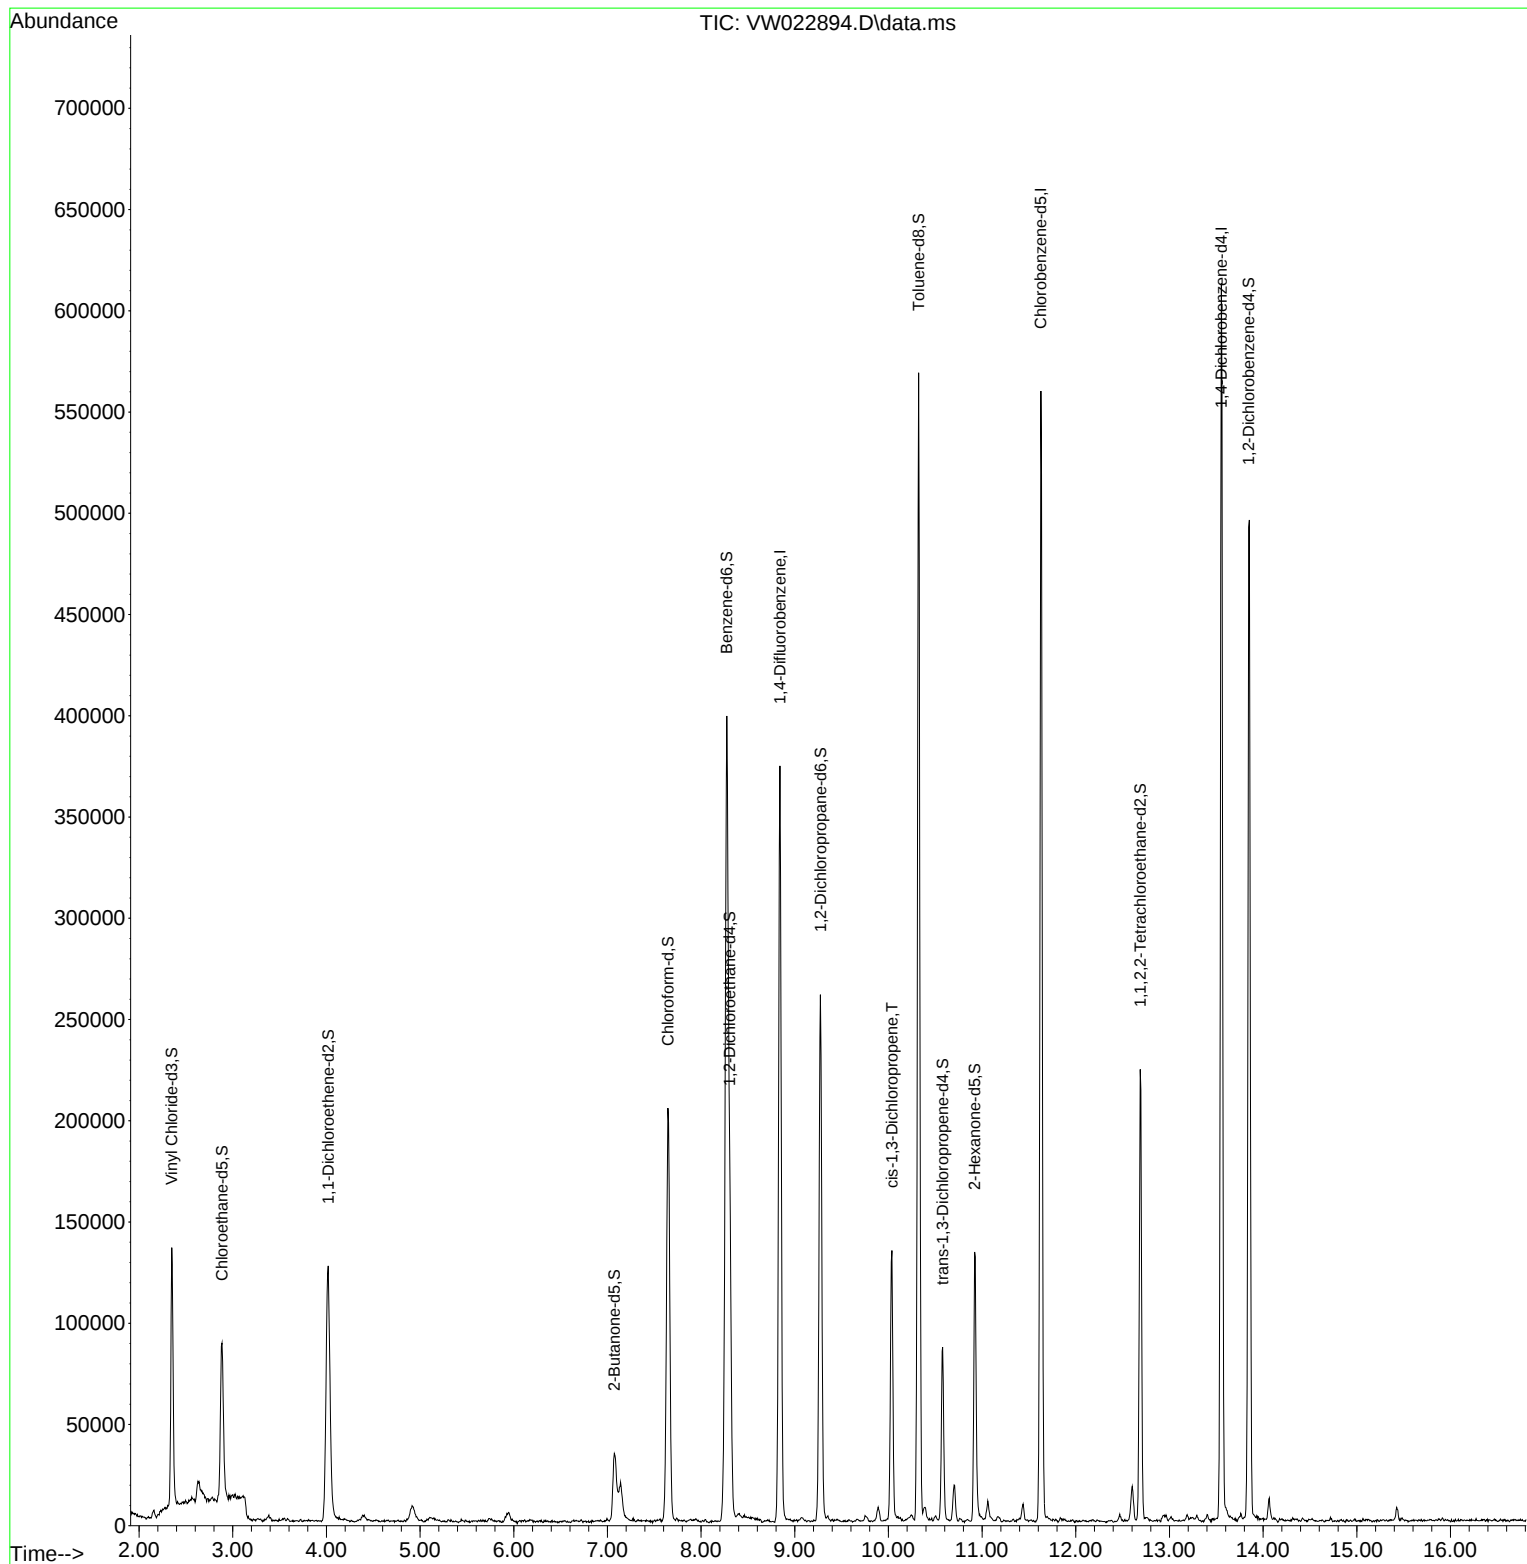

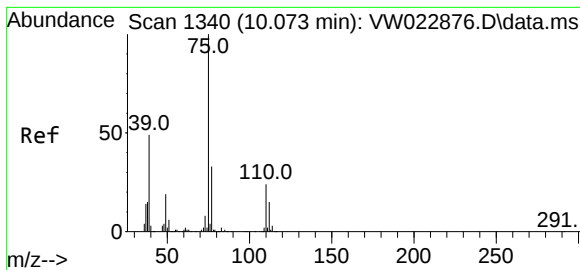

#39
 cis-1,3-Dichloropropene
 Concen: 0.589 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022894.D
 Acq: 06 May 2022 16:55

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3897
 Ion Ratio Lower Upper
 75 100
 77 49.4 22.1 41.1#

