

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022895.D
 Acq On : 06 May 2022 17:19
 Operator : SY/VA
 Sample : N2709-18
 Misc : 5.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 07 00:07:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 00:02:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	330306	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	308013	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	122837	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	136820	20.190	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.760%
7) Chloroethane-d5	2.885	69	102676	23.289	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.160%
11) 1,1-Dichloroethene-d2	4.214	63	123	0.014	ug/L	0.20
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.040%#
21) 2-Butanone-d5	7.074	46	58962	45.761	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.520%
24) Chloroform-d	7.647	84	236308	24.419	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.680%
26) 1,2-Dichloroethane-d4	8.384	65	225	0.042	ug/L	0.08
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.160%#
32) Benzene-d6	8.275	84	442982	24.952	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.800%
36) 1,2-Dichloropropane-d6	9.274	67	137790	27.630	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.520%
41) Toluene-d8	10.323	98	392511	22.887	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.560%
43) trans-1,3-Dichloroprop...	10.579	79	50436	21.965	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.840%
47) 2-Hexanone-d5	10.927	63	45907	48.221	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.440%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	125821	27.068	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.280%
66) 1,2-Dichlorobenzene-d4	13.853	152	107084	24.938	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.760%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	4314	0.634	ug/L #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022895.D
Acq On : 06 May 2022 17:19
Operator : SY/VA
Sample : N2709-18
Misc : 5.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 07 00:07:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 00:02:41 2022
Response via : Initial Calibration

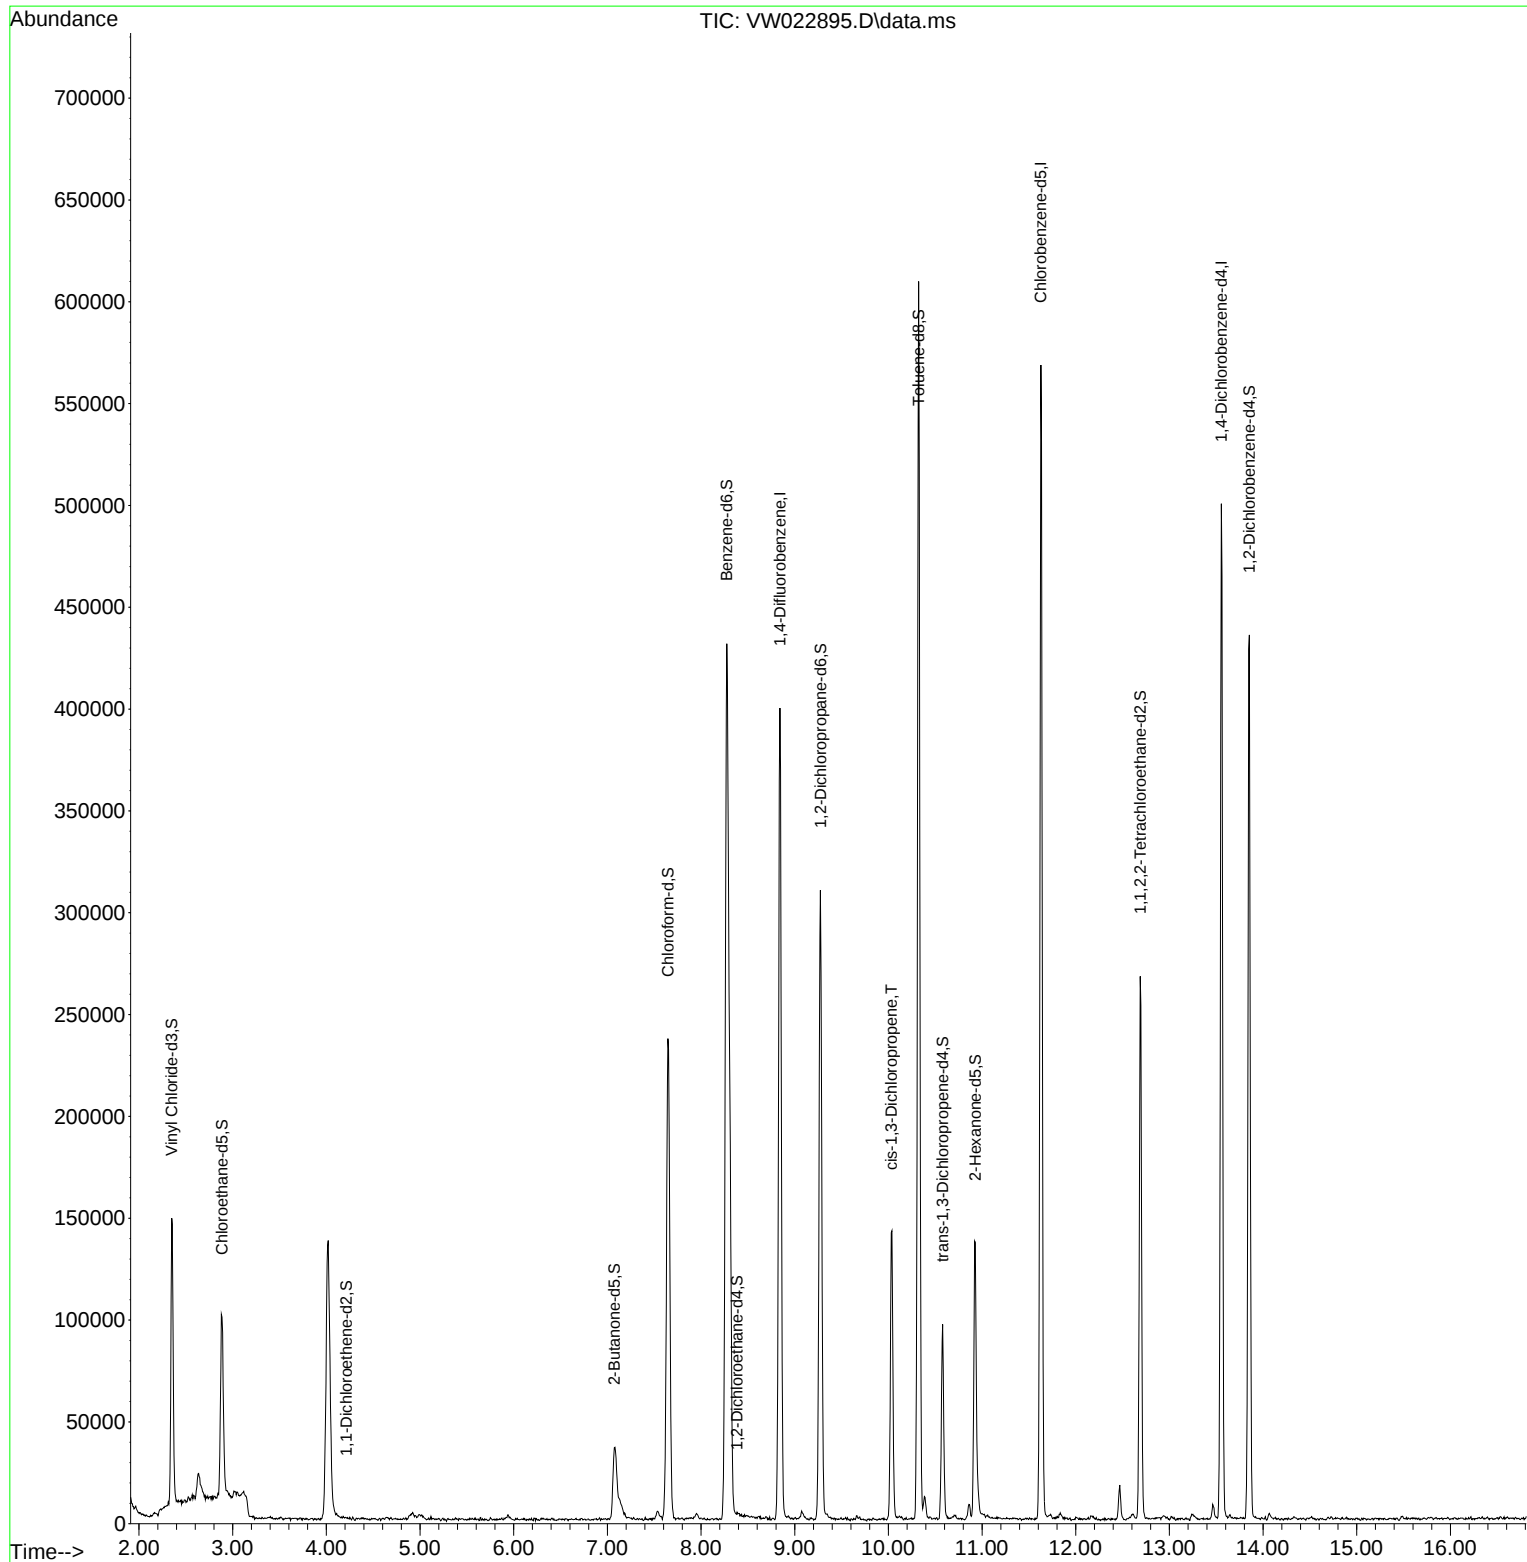

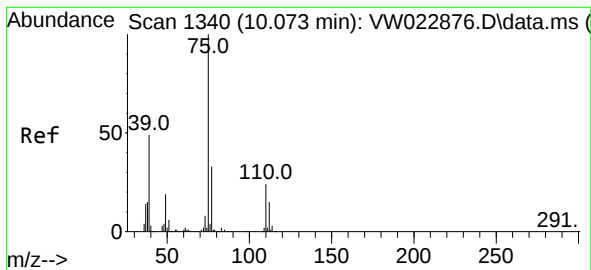

#39
 cis-1,3-Dichloropropene
 Concen: 0.634 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW022895.D
 Acq: 06 May 2022 17:19

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4314
 Ion Ratio Lower Upper
 75 100
 77 43.5 22.1 41.1#

