

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022896.D
 Acq On : 06 May 2022 17:43
 Operator : SY/VA
 Sample : N2711-01
 Misc : 5.32g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 07 00:07:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 00:02:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	351140	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	340797	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	166854	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	126047	17.496	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.000%
7) Chloroethane-d5	2.885	69	99199	21.165	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.680%
11) 1,1-Dichloroethene-d2	4.013	63	124025	13.324	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.280%
21) 2-Butanone-d5	7.074	46	71282	52.041	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.080%
24) Chloroform-d	7.653	84	226606	22.027	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.120%
26) 1,2-Dichloroethane-d4	8.305	65	134154	23.776	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.120%
32) Benzene-d6	8.275	84	427775	21.777	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.120%
36) 1,2-Dichloropropane-d6	9.274	67	129595	23.486	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.960%
41) Toluene-d8	10.323	98	378618	19.953	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.800%
43) trans-1,3-Dichloroprop...	10.579	79	51541	20.287	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.160%
47) 2-Hexanone-d5	10.920	63	58360	55.404	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.800%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	129099	25.102	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.400%
66) 1,2-Dichlorobenzene-d4	13.853	152	133930	22.962	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.840%
Target Compounds					Qvalue	
48) 2-Hexanone	10.920	43	7754	3.790	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022896.D
Acq On : 06 May 2022 17:43
Operator : SY/VA
Sample : N2711-01
Misc : 5.32g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 07 00:07:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 00:02:41 2022
Response via : Initial Calibration

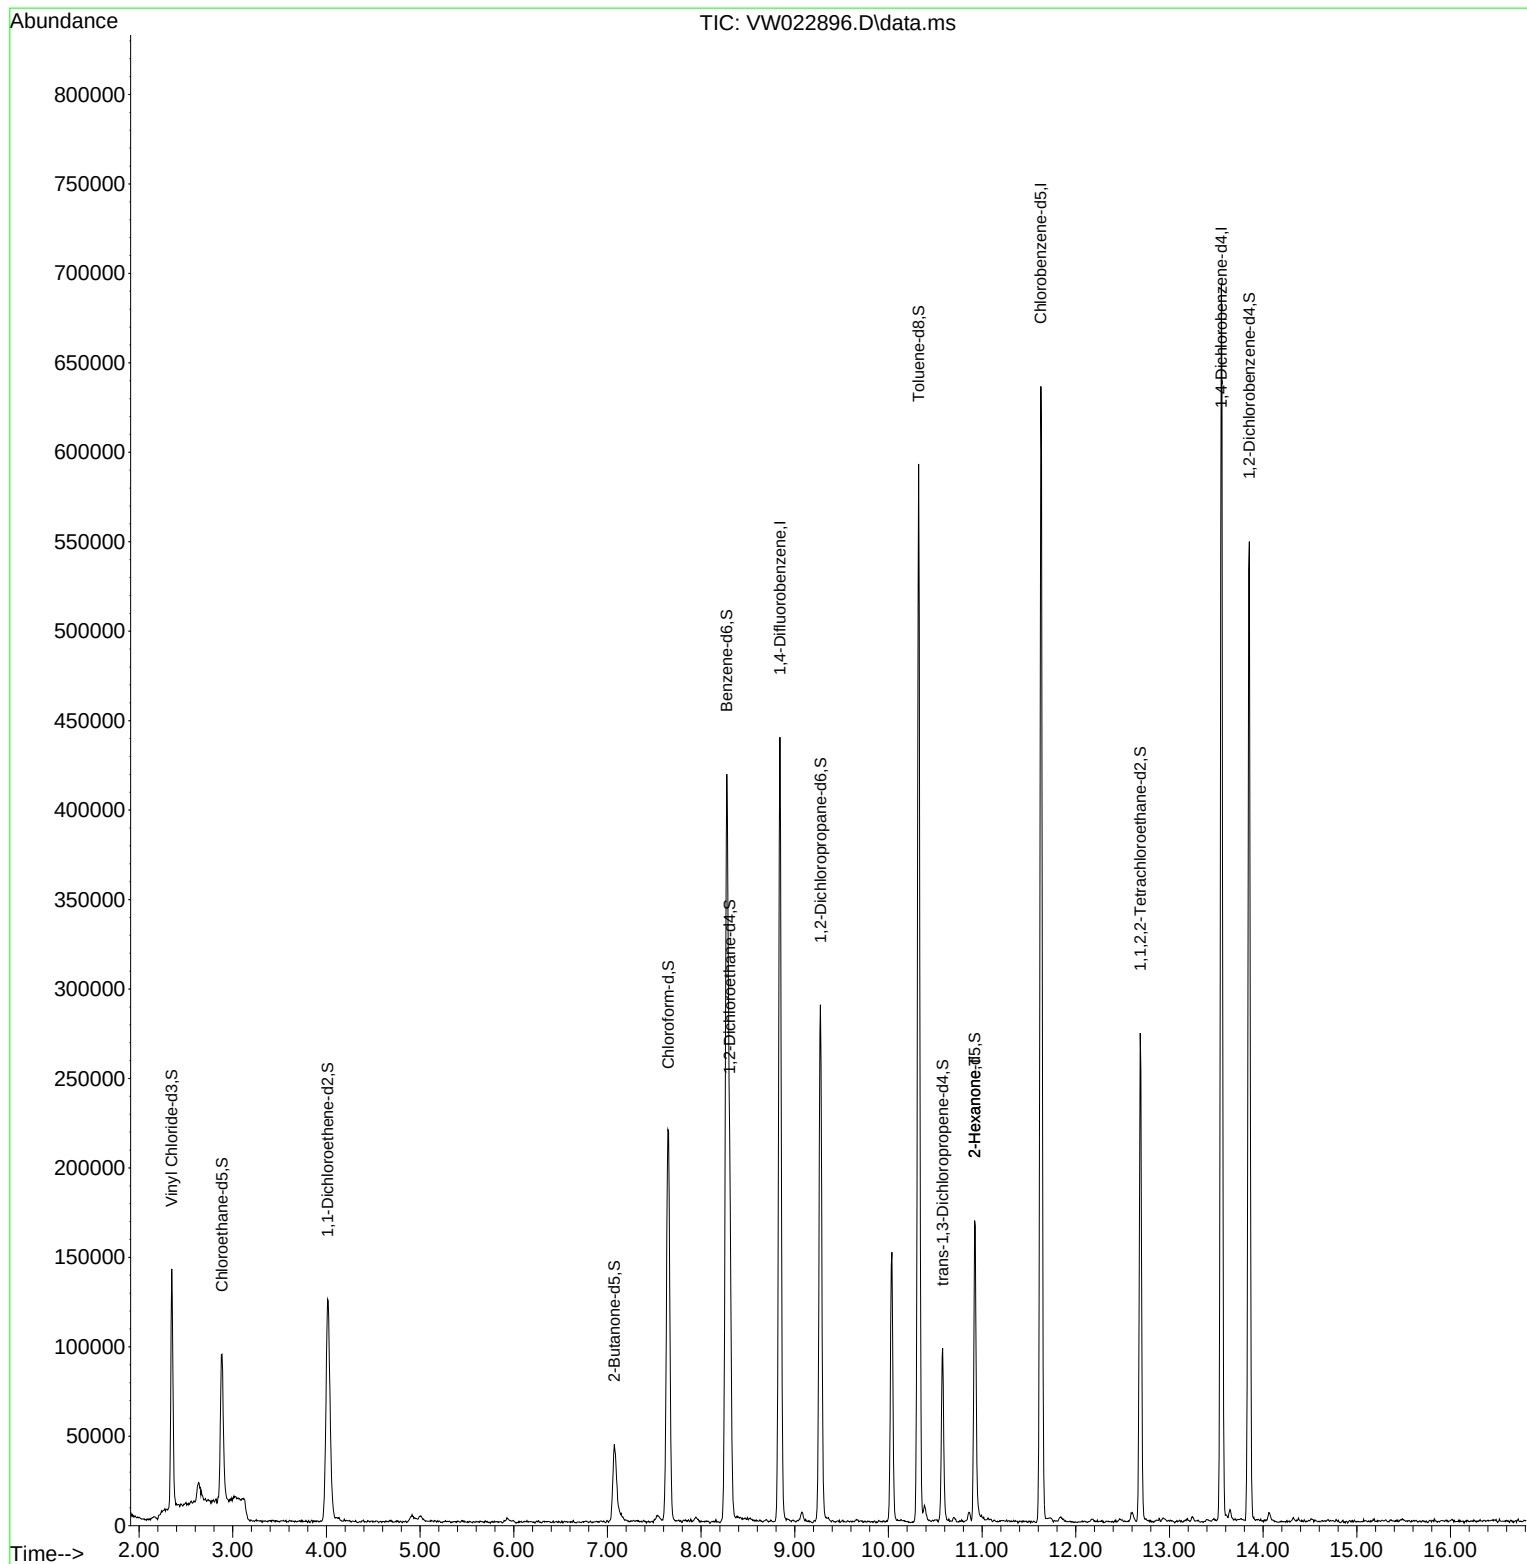

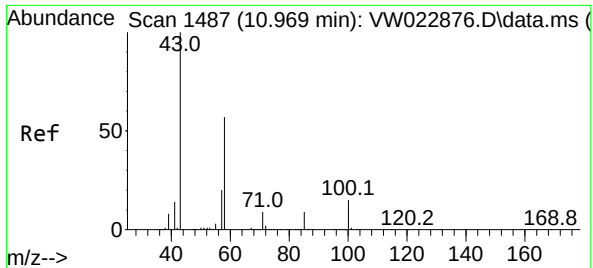

#48
 2-Hexanone
 Concen: 3.790 ug/L
 RT: 10.920 min Scan# 14
 Delta R.T. -0.049 min
 Lab File: VW022896.D
 Acq: 06 May 2022 17:43

Instrument :
 MSVOA_W
 ClientSampleId :

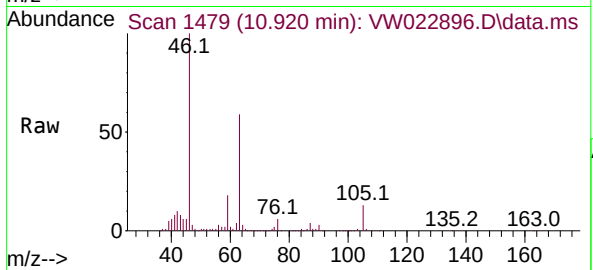

Tgt Ion: 43 Resp: 7754
 Ion Ratio Lower Upper
 43 100
 58 28.7 45.9 68.9#
 57 30.2 16.2 24.2#
 100 2.0 10.7 16.1#

