

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022899.D
 Acq On : 06 May 2022 18:55
 Operator : SY/VA
 Sample : N2638-24
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 07 00:07:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 00:02:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	276205	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	270543	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	135500	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	112521	19.856	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.440%
7) Chloroethane-d5	2.885	69	85589	23.216	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.880%
11) 1,1-Dichloroethene-d2	4.013	63	109007	14.887	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.560%
21) 2-Butanone-d5	7.074	46	50778	47.129	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.260%
24) Chloroform-d	7.647	84	181567	22.437	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.760%
26) 1,2-Dichloroethane-d4	8.305	65	102688	23.137	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.560%
32) Benzene-d6	8.275	84	344470	22.090	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.360%
36) 1,2-Dichloropropane-d6	9.274	67	102602	23.423	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.680%
41) Toluene-d8	10.323	98	328535	21.810	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.240%
43) trans-1,3-Dichloroprop...	10.579	79	39040	19.356	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.440%
47) 2-Hexanone-d5	10.921	63	40396	48.309	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.620%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	95496	23.390	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	110836	23.400	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.600%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4076	0.682	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022899.D
Acq On : 06 May 2022 18:55
Operator : SY/VA
Sample : N2638-24
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 07 00:07:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 00:02:41 2022
Response via : Initial Calibration

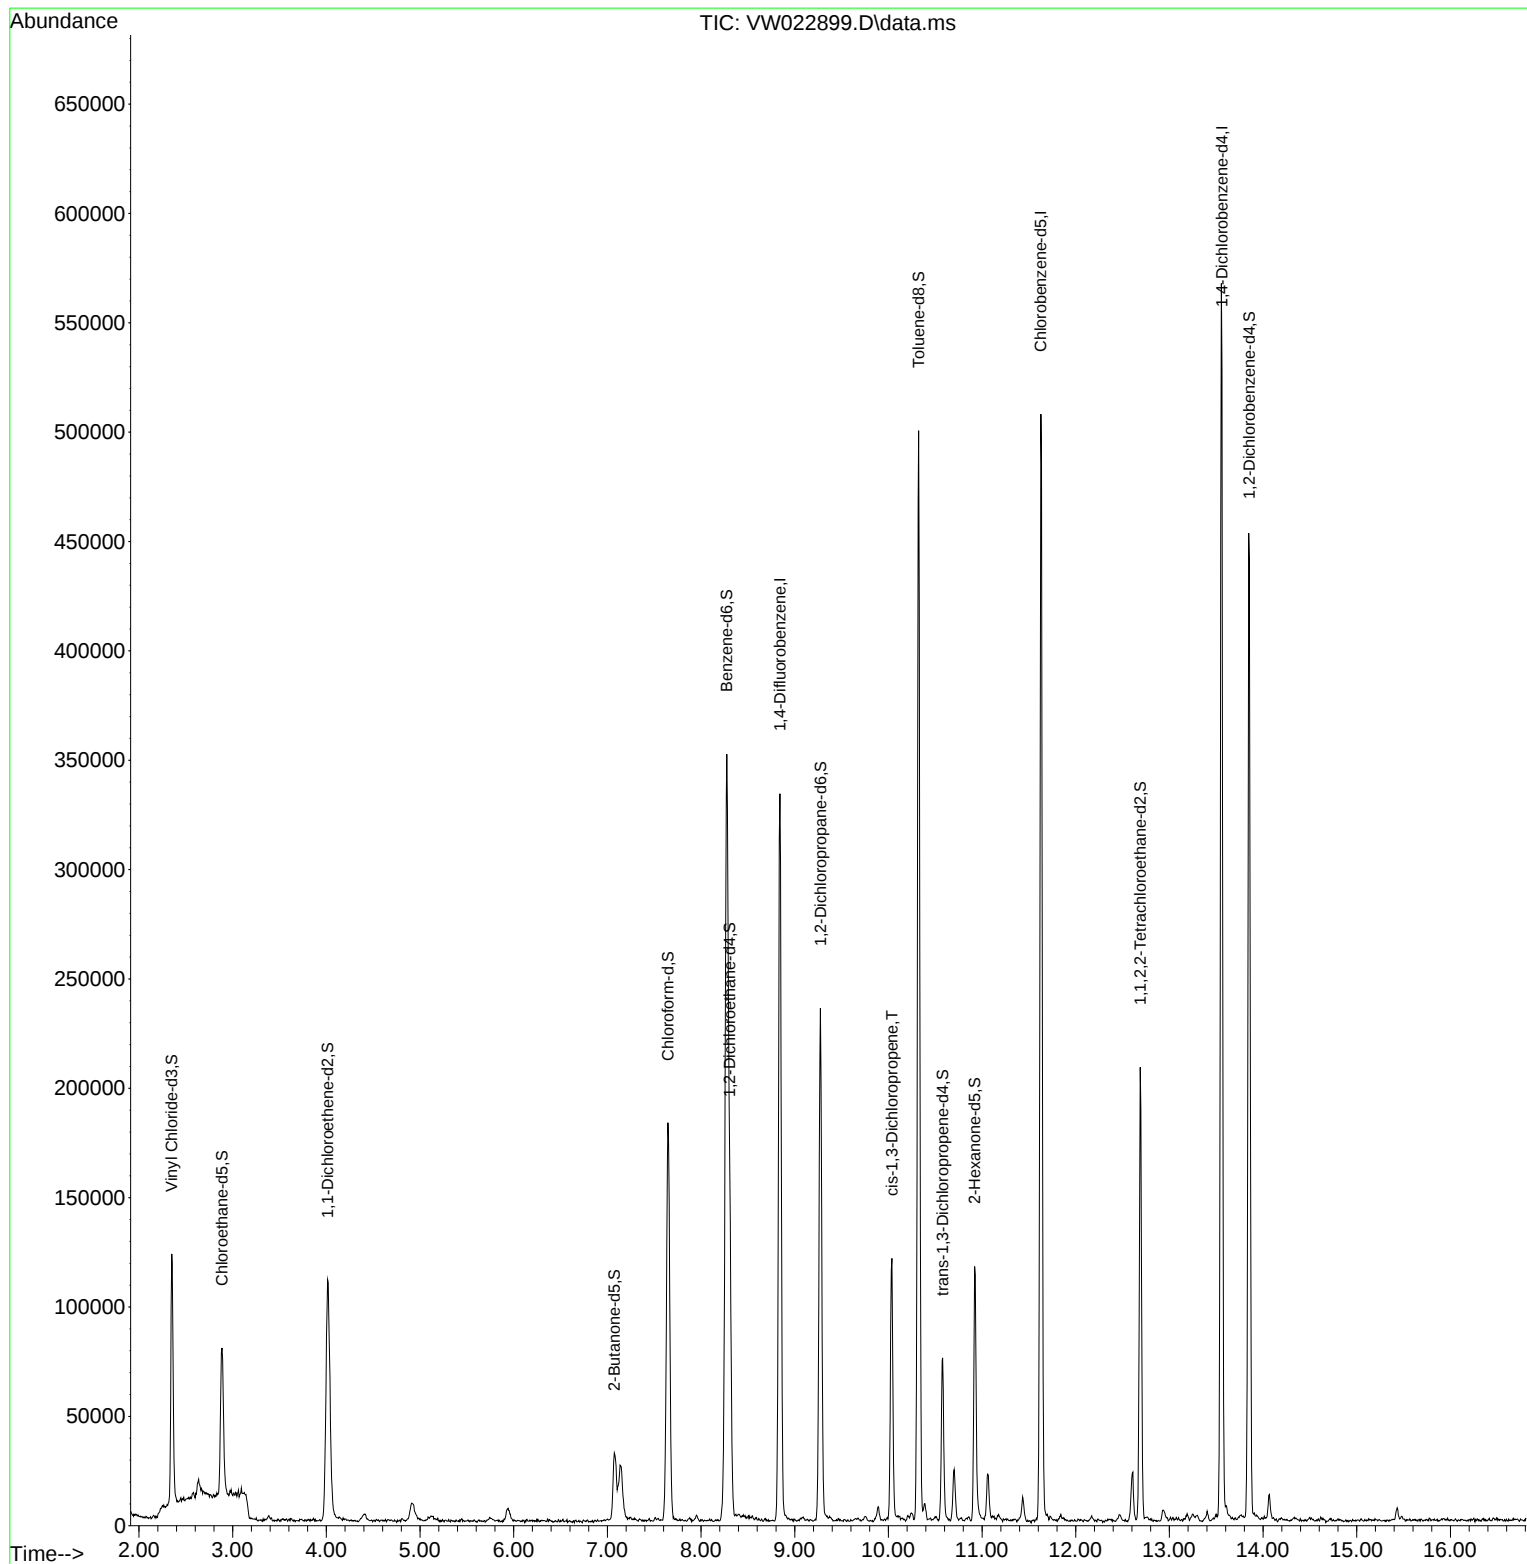

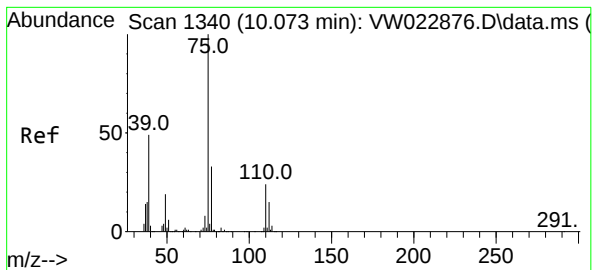

#39
 cis-1,3-Dichloropropene
 Concen: 0.682 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022899.D
 Acq: 06 May 2022 18:55

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4076
 Ion Ratio Lower Upper
 75 100
 77 38.6 22.1 41.1

