




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022902.D
 Acq On : 06 May 2022 20:56
 Operator : SY/VA
 Sample : N2714-02
 Misc : 4.39g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X5

Manual IntegrationsAPPROVED

Quant Time: May 07 03:05:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 01:54:32 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/07/2022
 Supervised By :Mahesh Dadoda 05/10/2022

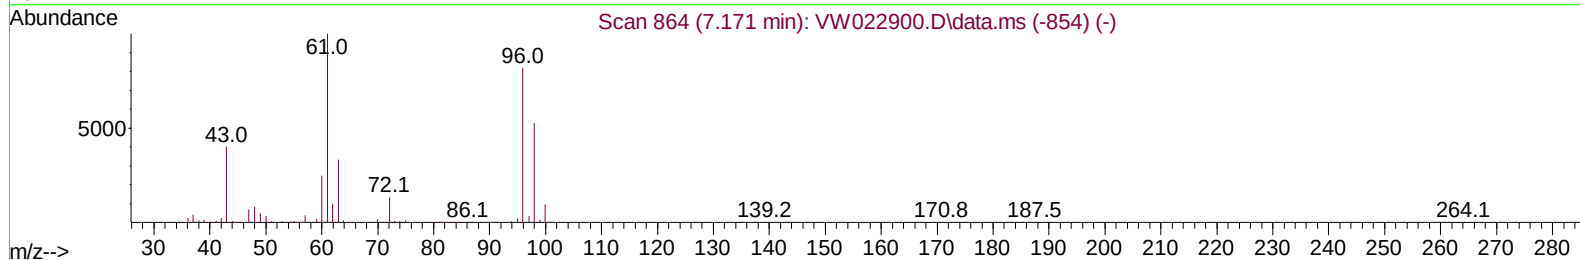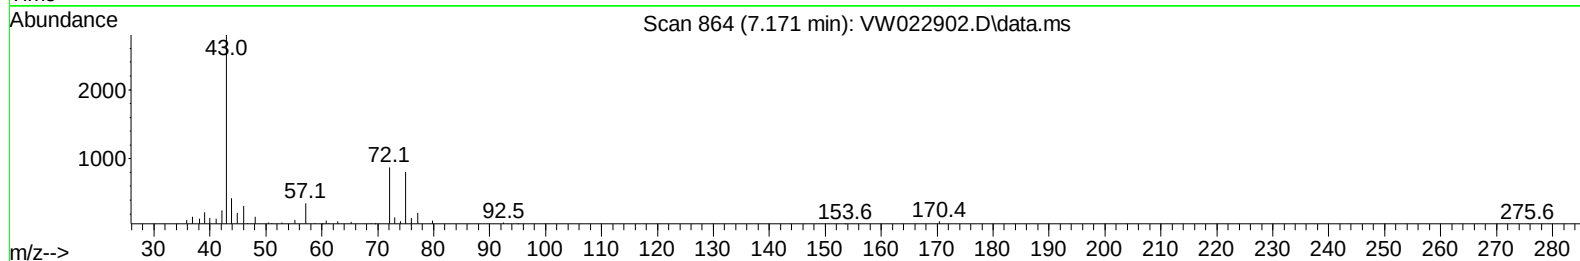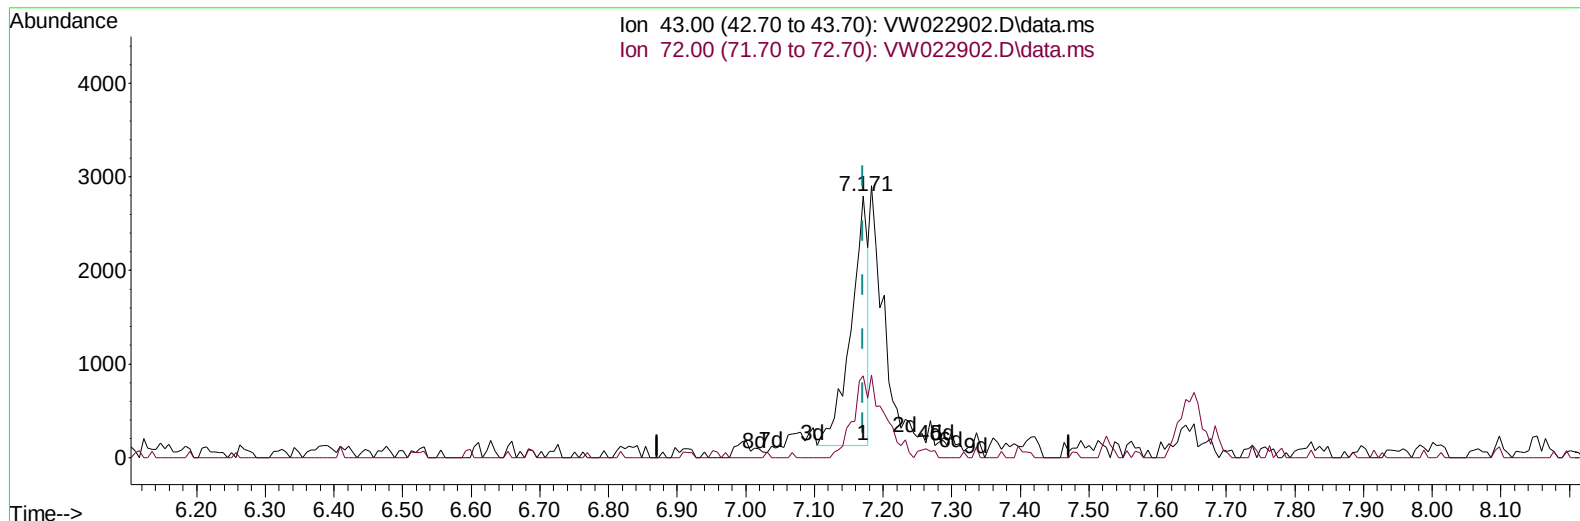

TIC: VW022902.D\data.ms

(22) 2-Butanone (T)

7.171min (+ 0.000) 3.58 ug/L

response 4602

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.20	9.41#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022902.D
 Acq On : 06 May 2022 20:56
 Operator : SY/VA
 Sample : N2714-02
 Misc : 4.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X5

Manual IntegrationsAPPROVED

Quant Time: May 07 03:05:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 01:54:32 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/07/2022
 Supervised By :Mahesh Dadoda 05/10/2022

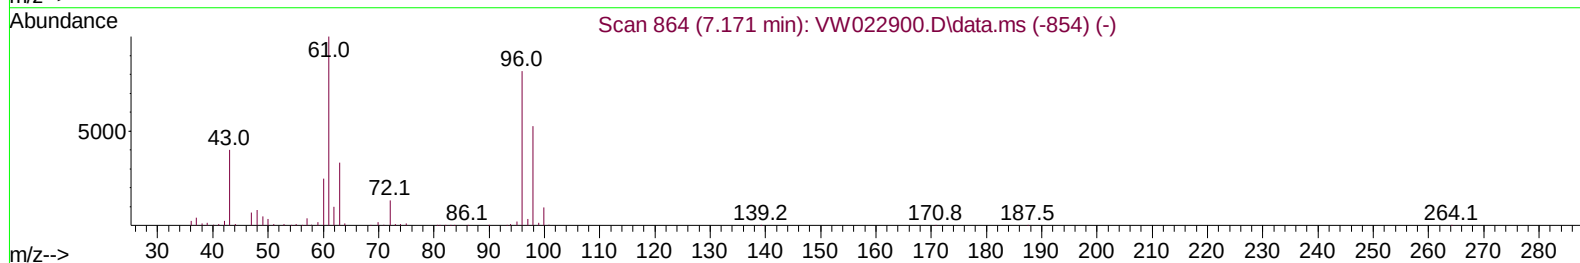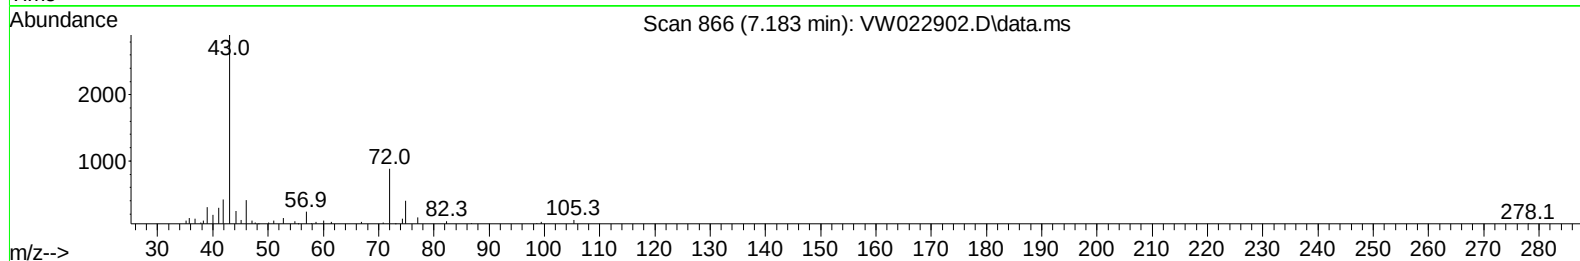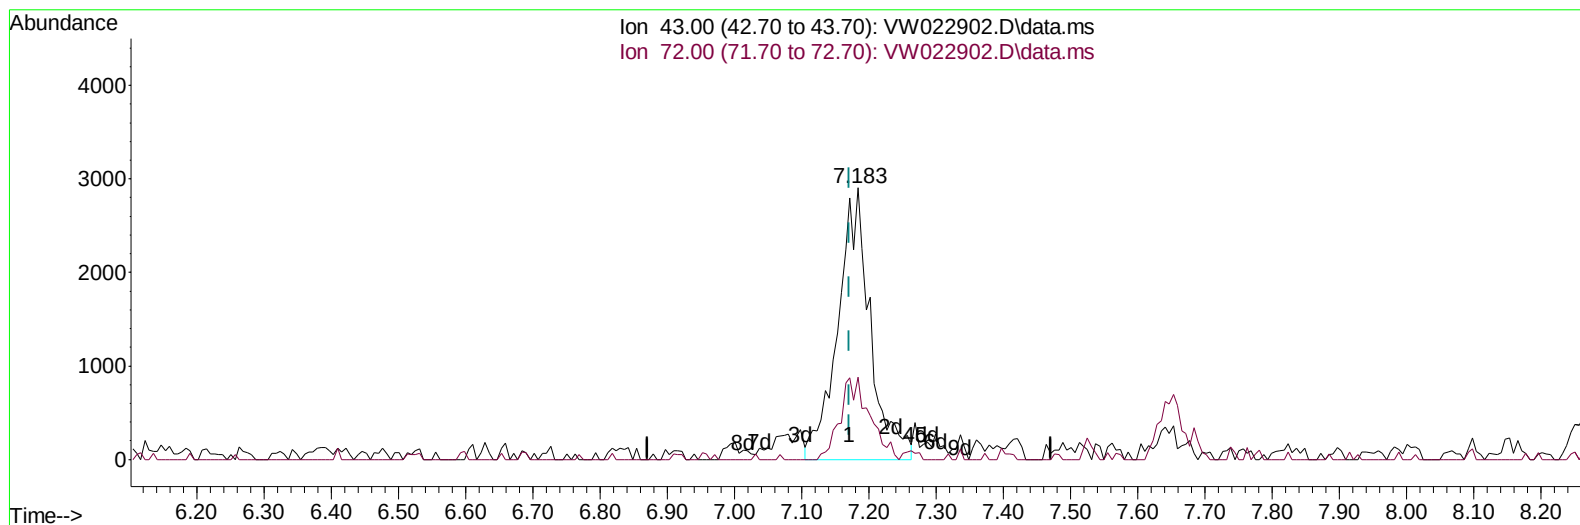

TIC: VW022902.D\data.ms

(22) 2-Butanone (T)

7.183min (+ 0.013) 7.56 ug/L m

response 9723

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	30.20	4.45#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022902.D
 Acq On : 06 May 2022 20:56
 Operator : SY/VA
 Sample : N2714-02
 Misc : 4.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X5

Manual IntegrationsAPPROVED

Quant Time: May 07 03:05:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 01:54:32 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/07/2022
 Supervised By :Mahesh Dadoda 05/10/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	314900	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	282525	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93601	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	113150	17.514	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	70.040%	
7) Chloroethane-d5	2.885	69	90835	21.611	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	86.440%	
11) 1,1-Dichloroethene-d2	4.013	63	114269	13.688	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	54.760%	
21) 2-Butanone-d5	7.080	46	50995	41.514	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	83.020%	
24) Chloroform-d	7.647	84	203410	22.048	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.200%	
26) 1,2-Dichloroethane-d4	8.305	65	112881	22.308	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	89.240%	
32) Benzene-d6	8.275	84	373823	22.956	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	91.840%	
36) 1,2-Dichloropropane-d6	9.275	67	110715	24.203	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	96.800%	
41) Toluene-d8	10.323	98	329052	20.917	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	83.680%	
43) trans-1,3-Dichloroprop...	10.573	79	33585	15.946	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	63.800%	
47) 2-Hexanone-d5	10.921	63	38691	44.307	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	88.620%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	89707	21.040	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	84.160%	
66) 1,2-Dichlorobenzene-d4	13.853	152	73939	22.598	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	90.400%	
Target Compounds						
13) Acetone	4.123	43	28250	30.718	ug/L	98
22) 2-Butanone	7.183	43	9723m	7.560	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022902.D
Acq On : 06 May 2022 20:56
Operator : SY/VA
Sample : N2714-02
Misc : 4.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW2X5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/07/2022
Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 07 03:05:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 01:54:32 2022
Response via : Initial Calibration

