




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022907.D
 Acq On : 06 May 2022 22:57
 Operator : SY/VA
 Sample : N2711-06
 Misc : 6.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL97

Manual IntegrationsAPPROVED

Quant Time: May 07 03:06:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 01:54:32 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/07/2022
 Supervised By :Mahesh Dadoda 05/10/2022

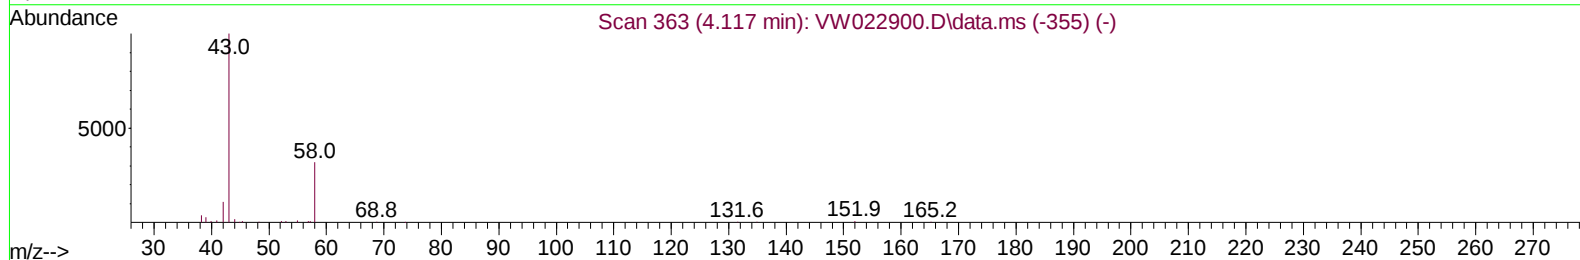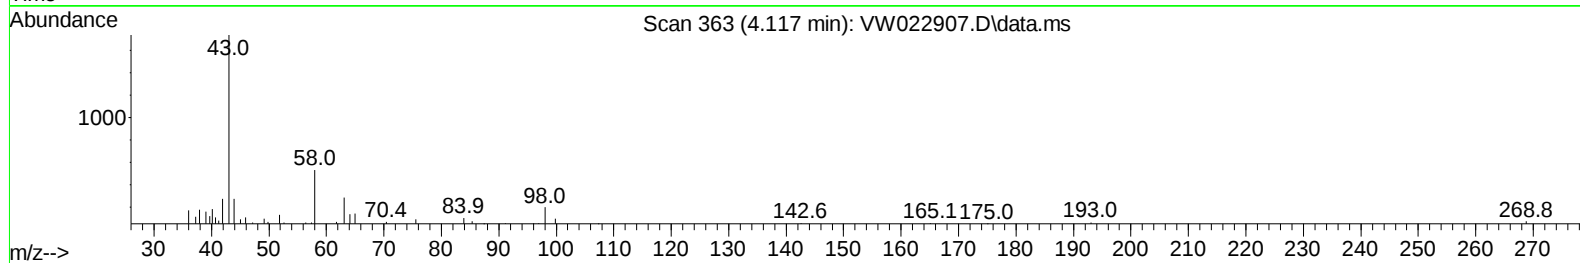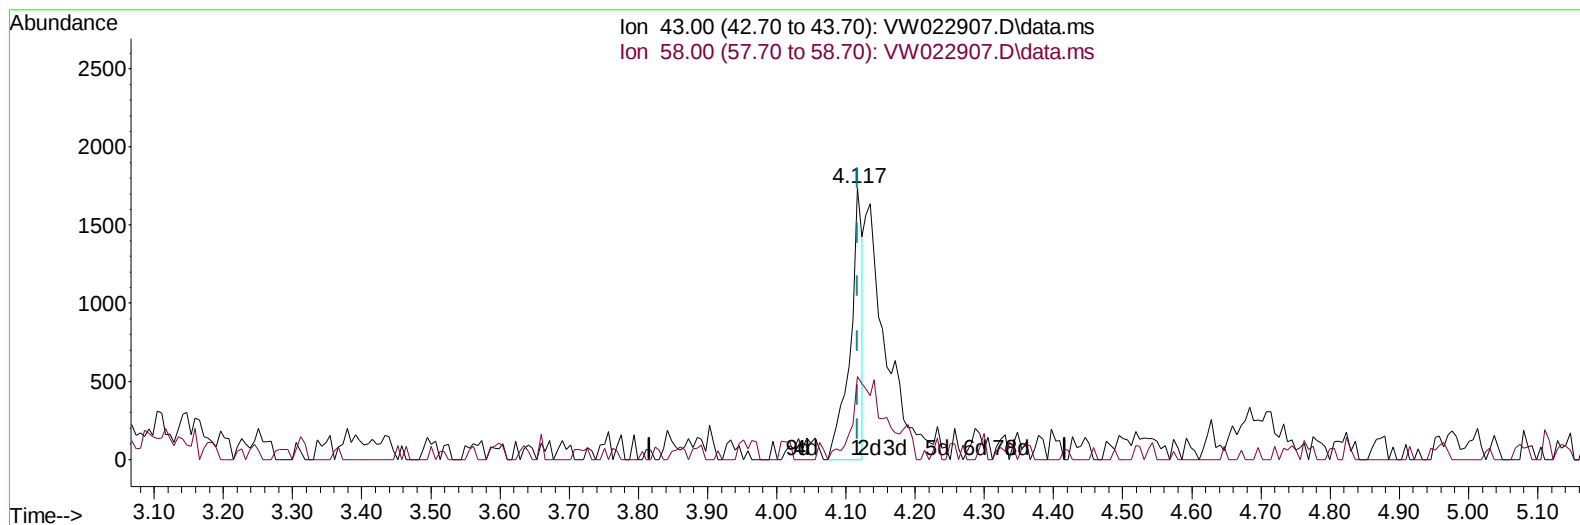

TIC: VW022907.D\data.ms

(13) Acetone (T)

4.117min (-0.000) 2.38 ug/L

response 2093

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	41.14
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022907.D
 Acq On : 06 May 2022 22:57
 Operator : SY/VA
 Sample : N2711-06
 Misc : 6.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL97

Manual IntegrationsAPPROVED

Quant Time: May 07 03:06:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 01:54:32 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/07/2022
 Supervised By :Mahesh Dadoda 05/10/2022

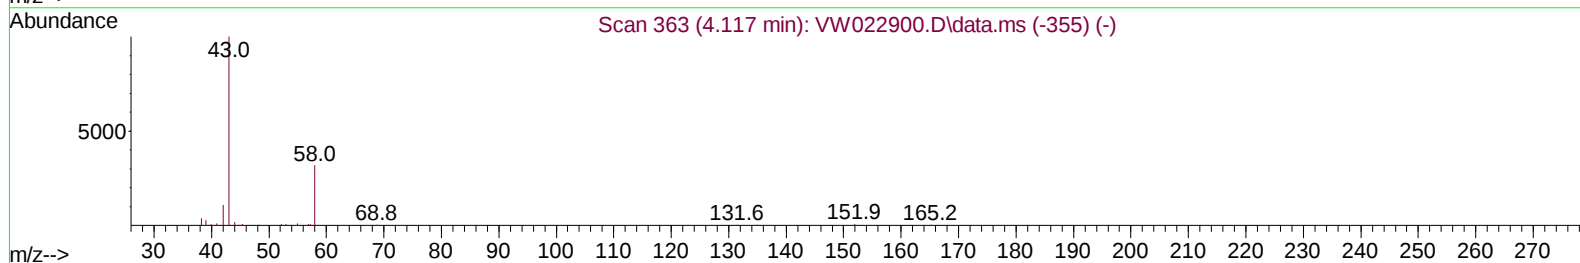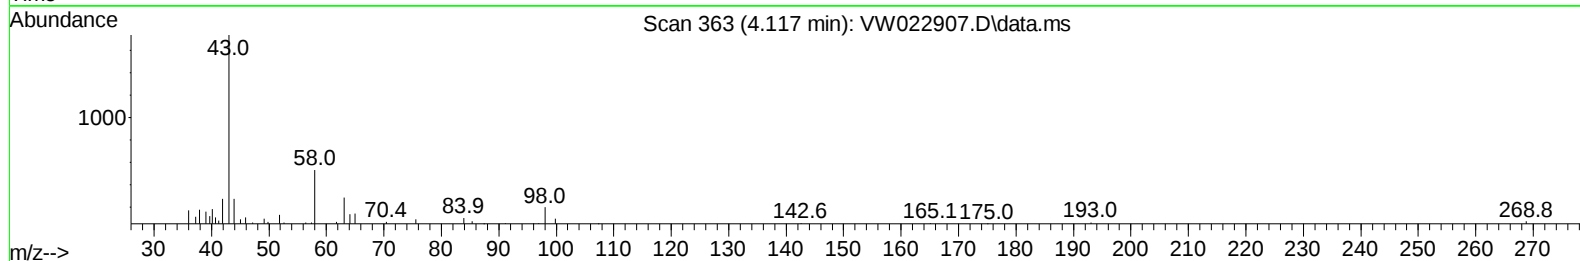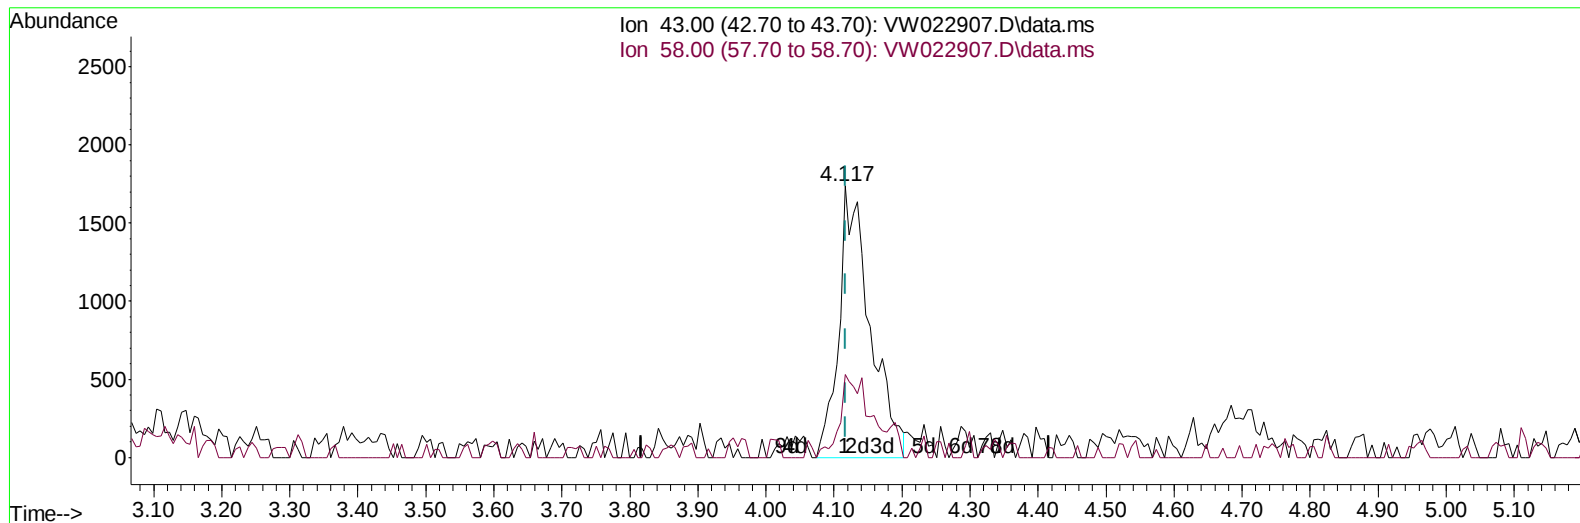

TIC: VW022907.D\data.ms

(13) Acetone (T)

4.117min (-0.000) 6.26 ug/L m

response 5509

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	15.63
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022907.D
 Acq On : 06 May 2022 22:57
 Operator : SY/VA
 Sample : N2711-06
 Misc : 6.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXL97

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/07/2022
 Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 07 03:06:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 01:54:32 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		301227	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117		294746	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		139814	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		102774	16.630	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	66.520%	
7) Chloroethane-d5	2.885	69		83837	20.852	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.400%	
11) 1,1-Dichloroethene-d2	4.019	63		105722	13.239	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	52.960%	
21) 2-Butanone-d5	7.079	46		57949	49.317	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	98.640%	
24) Chloroform-d	7.646	84		195907	22.198	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	88.800%	
26) 1,2-Dichloroethane-d4	8.305	65		113525	23.454	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	93.800%	
32) Benzene-d6	8.274	84		360784	21.236	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	84.960%	
36) 1,2-Dichloropropane-d6	9.274	67		111002	23.260	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	93.040%	
41) Toluene-d8	10.323	98		330461	20.136	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	80.560%	
43) trans-1,3-Dichloroprop...	10.579	79		43646	19.863	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	79.440%	
47) 2-Hexanone-d5	10.920	63		48107	52.806	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	105.620%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		107901	24.258	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	97.040%	
66) 1,2-Dichlorobenzene-d4	13.853	152		114787	23.486	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	93.960%	
Target Compounds							
13) Acetone	4.117	43		5509m	6.262	ug/L	
46) Tetrachloroethene	10.859	164		6541	1.823	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022907.D
Acq On : 06 May 2022 22:57
Operator : SY/VA
Sample : N2711-06
Misc : 6.10g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXL97

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/07/2022
Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 07 03:06:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 01:54:32 2022
Response via : Initial Calibration

