




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022909.D
 Acq On : 06 May 2022 23:45
 Operator : SY/VA
 Sample : N2711-08
 Misc : 3.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLA0

Manual IntegrationsAPPROVED

Quant Time: May 07 03:07:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 01:54:32 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/07/2022
 Supervised By :Mahesh Dadoda 05/10/2022

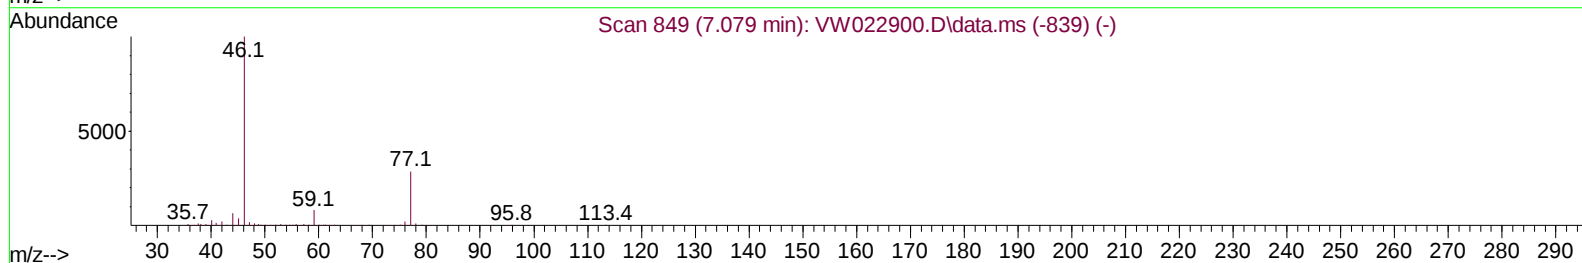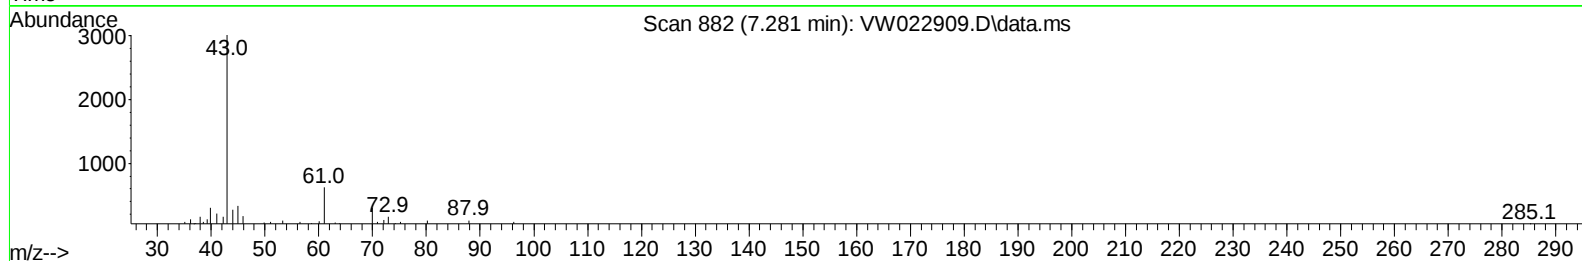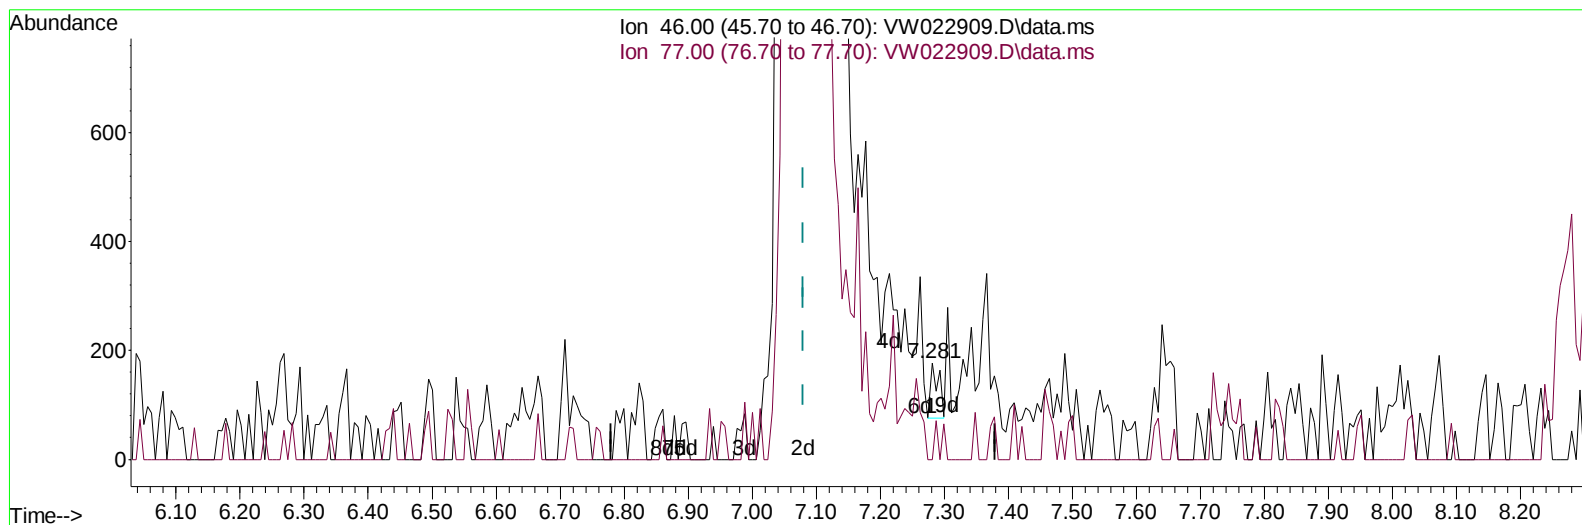

TIC: VW022909.D\data.ms

(21) 2-Butanone-d5 (S)

7.281min (+ 0.201) 0.08 ug/L

response 88

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	29.55
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022909.D
Acq On : 06 May 2022 23:45
Operator : SY/VA
Sample : N2711-08
Misc : 3.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXLA0

Manual IntegrationsAPPROVED

Quant Time: May 07 03:07:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 01:54:32 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/07/2022
Supervised By :Mahesh Dadoda 05/10/2022

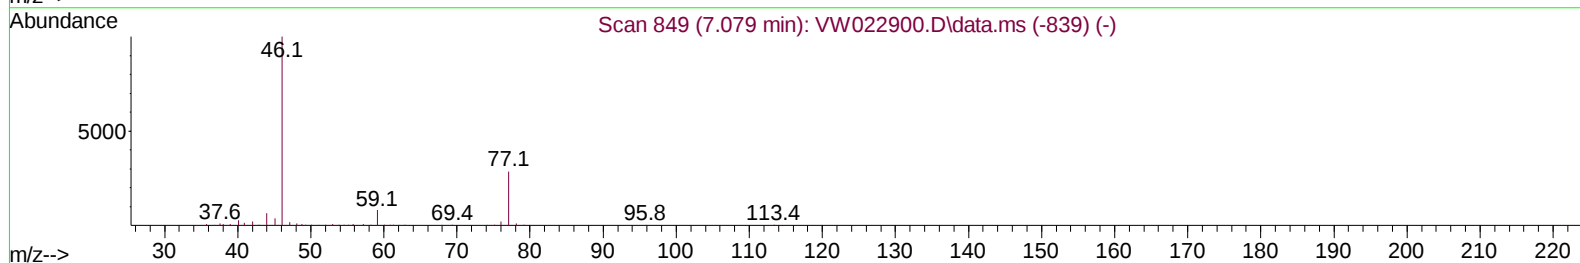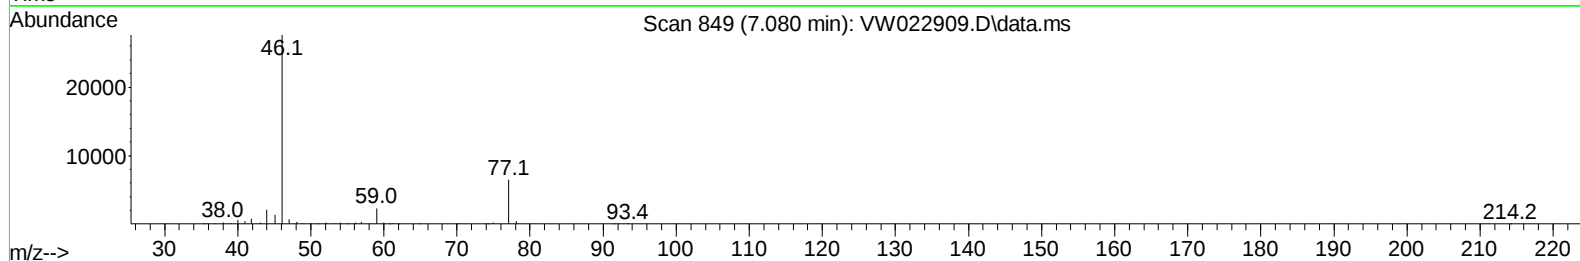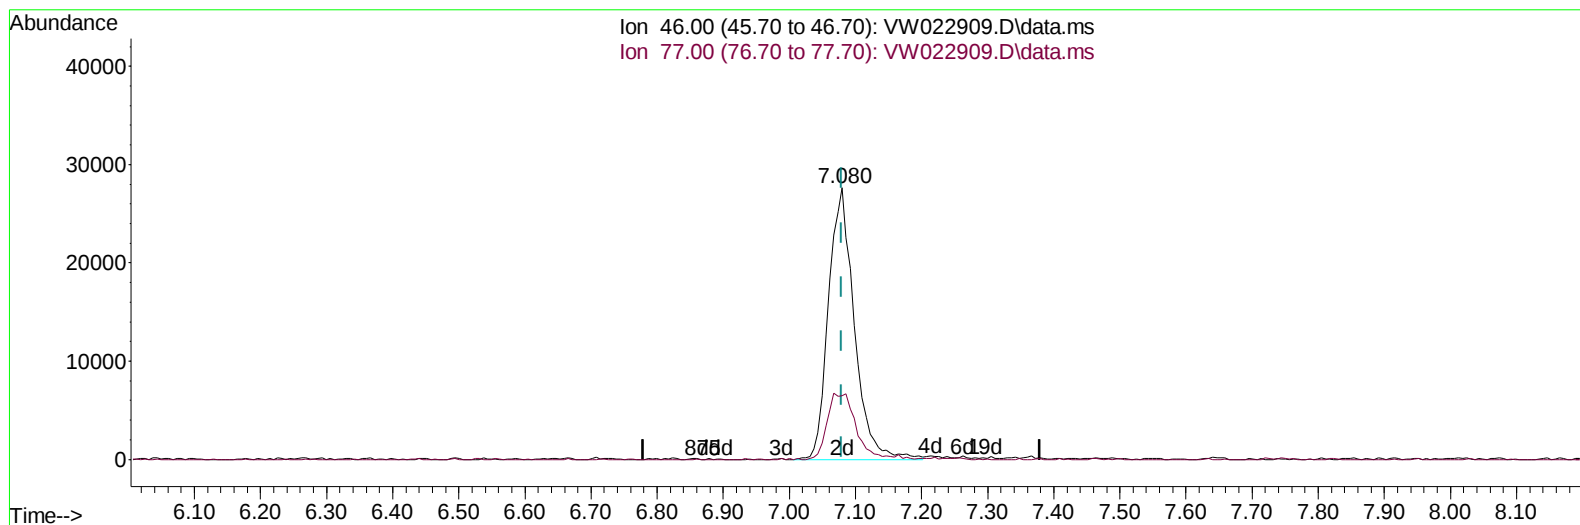

TIC: VW022909.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.000) 64.93 ug/L m

response 75042

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.03#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022909.D
 Acq On : 06 May 2022 23:45
 Operator : SY/VA
 Sample : N2711-08
 Misc : 3.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXLA0

Manual IntegrationsAPPROVED

Quant Time: May 07 03:07:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 01:54:32 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/07/2022
 Supervised By :Mahesh Dadoda 05/10/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		296302	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		304933	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		158568	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		99275	16.331	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	65.320%		
7) Chloroethane-d5	2.879	69		78580	19.869	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.480%		
11) 1,1-Dichloroethene-d2	4.013	63		99680	12.690	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	50.760%		
21) 2-Butanone-d5	7.080	46		75042m	64.925	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	129.860%		
24) Chloroform-d	7.653	84		207714	23.928	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	95.720%		
26) 1,2-Dichloroethane-d4	8.305	65		129737	27.249	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	109.000%		
32) Benzene-d6	8.275	84		381264	21.692	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	86.760%		
36) 1,2-Dichloropropane-d6	9.274	67		123784	25.072	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	100.280%		
41) Toluene-d8	10.323	98		350968	20.671	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	82.680%		
43) trans-1,3-Dichloroprop...	10.579	79		51420	22.619	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	90.480%		
47) 2-Hexanone-d5	10.920	63		59624	63.262	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	126.520%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		132996	28.901	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	115.600%		
66) 1,2-Dichlorobenzene-d4	13.853	152		130465	23.537	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	94.160%		
Target Compounds							
						Qvalue	
13) Acetone	4.135	43		3657	4.226	ug/L	87
46) Tetrachloroethene	10.866	164		3698	0.996	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022909.D
Acq On : 06 May 2022 23:45
Operator : SY/VA
Sample : N2711-08
Misc : 3.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXLA0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/07/2022
Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 07 03:07:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 01:54:32 2022
Response via : Initial Calibration

