

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
 Data File : VW022913.D
 Acq On : 07 May 2022 01:21
 Operator : SY/VA
 Sample : N2714-07
 Misc : 6.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X8

Quant Time: May 07 03:07:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 07 01:54:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	335784	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	306923	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	130018	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	109968	15.963	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.840%
7) Chloroethane-d5	2.885	69	82629	18.436	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.760%
11) 1,1-Dichloroethene-d2	4.013	63	108372	12.175	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.680%
21) 2-Butanone-d5	7.079	46	45843	34.999	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.000%
24) Chloroform-d	7.646	84	195631	19.886	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.560%
26) 1,2-Dichloroethane-d4	8.305	65	109440	20.283	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.120%
32) Benzene-d6	8.274	84	357982	20.235	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.960%
36) 1,2-Dichloropropane-d6	9.274	67	110141	22.164	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.640%
41) Toluene-d8	10.323	98	323528	18.931	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.720%
43) trans-1,3-Dichloroprop...	10.579	79	36371	15.896	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	63.600%
47) 2-Hexanone-d5	10.920	63	36819	38.812	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.620%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	94558	20.415	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.640%
66) 1,2-Dichlorobenzene-d4	13.853	152	90535	19.920	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.680%
Target Compounds						
					Qvalue	
14) Carbon disulfide	4.379	76	16807	1.425	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050622\
Data File : VW022913.D
Acq On : 07 May 2022 01:21
Operator : SY/VA
Sample : N2714-07
Misc : 6.67g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW2X8

Quant Time: May 07 03:07:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 07 01:54:32 2022
Response via : Initial Calibration

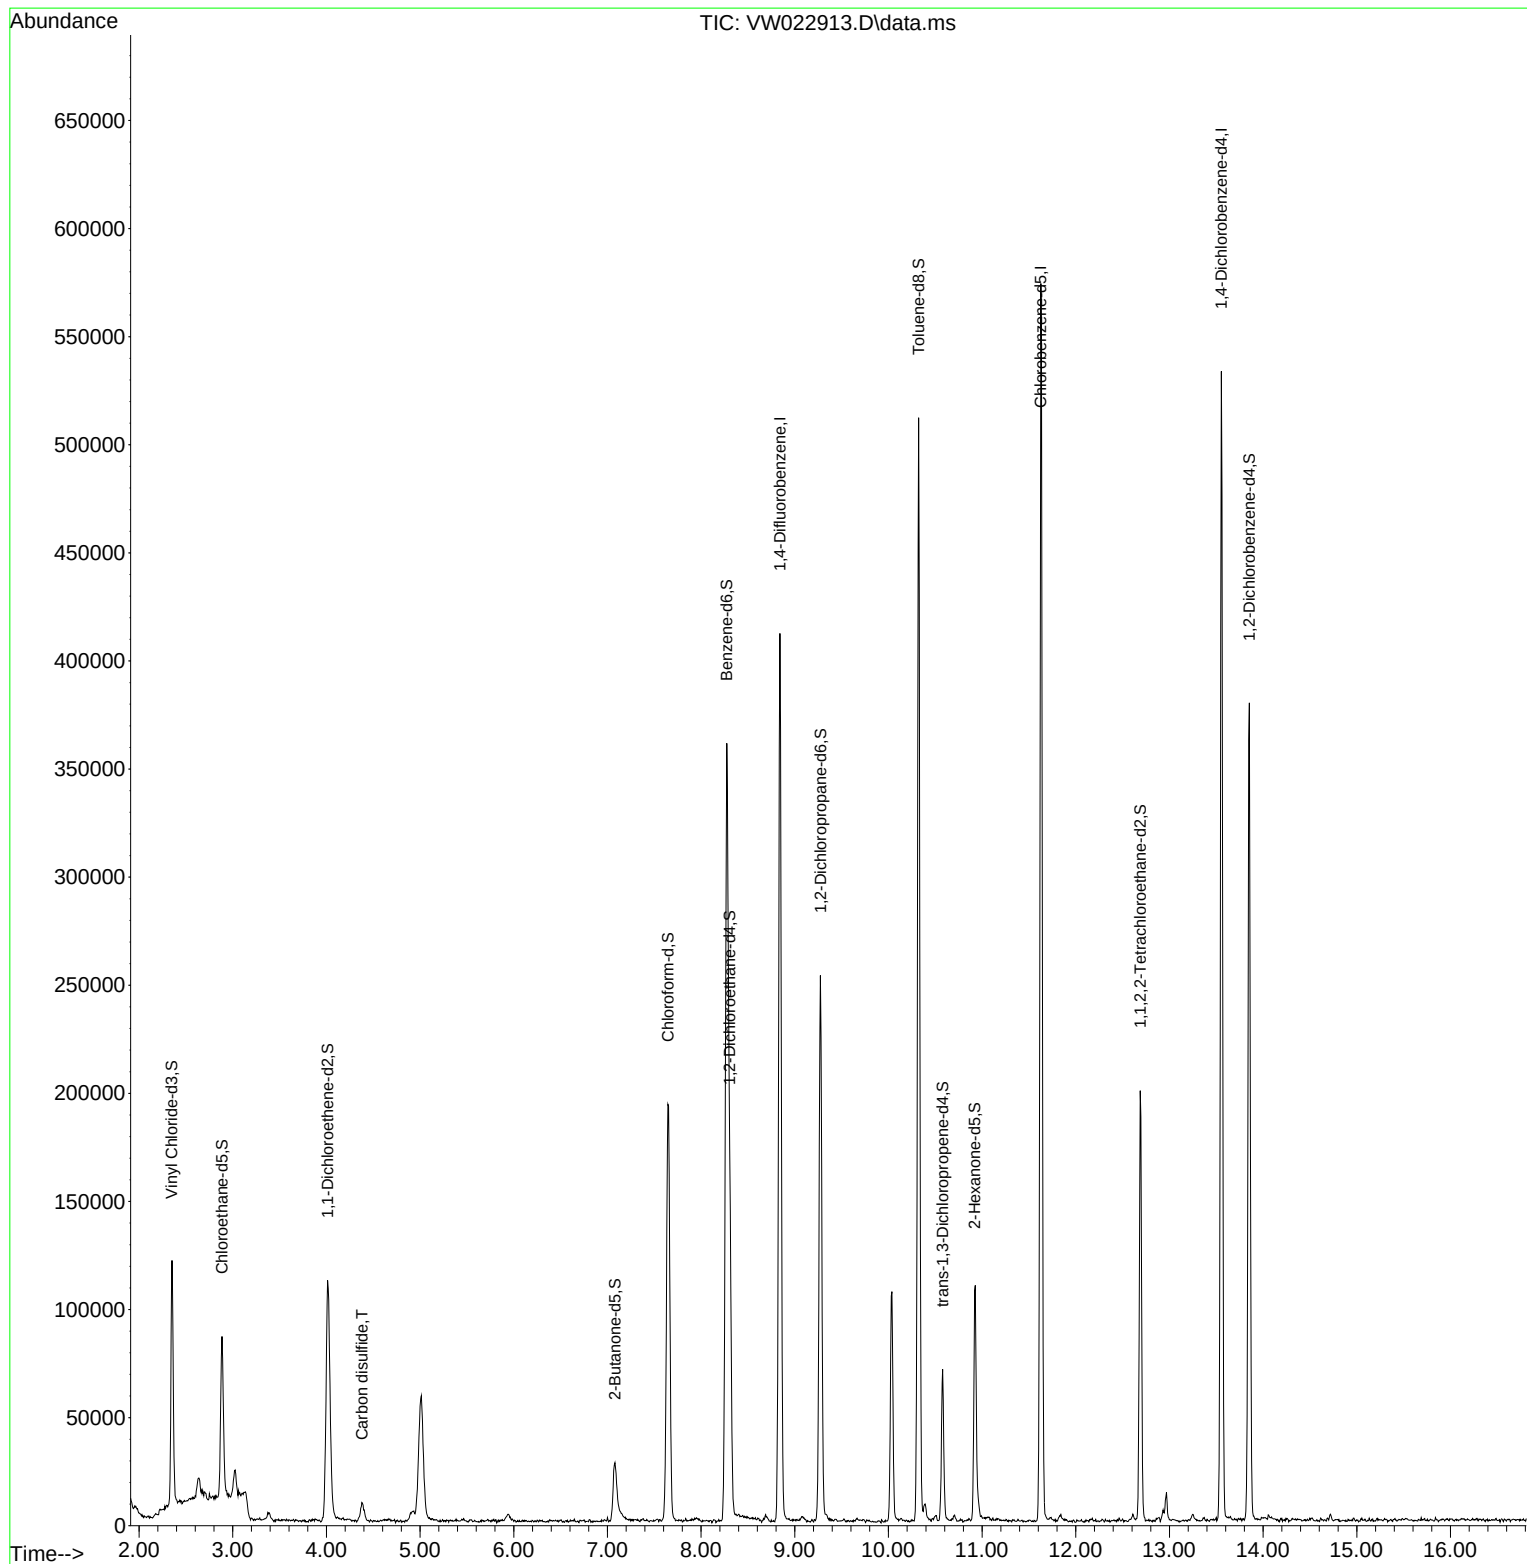

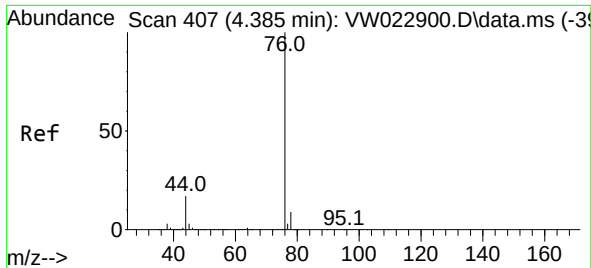

#14
Carbon disulfide
Concen: 1.425 ug/L
RT: 4.379 min Scan# 407
Delta R.T. -0.006 min
Lab File: VW022913.D
Acq: 07 May 2022 01:21

Instrument :
MSVOA_W
ClientSampleId :
EW2X8

Tgt Ion: 76 Resp: 16807
Ion Ratio Lower Upper
76 100
78 11.2 7.7 11.5

