

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
 Data File : VW025872.D
 Acq On : 08 May 2023 10:26
 Operator : SY/MD
 Sample : VW0508SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 09 02:56:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	599126	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	529827	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	214618	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	219388	25.841	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 103.360%			
7) Chloroethane-d5	2.899	69	165798	26.341	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 105.360%			
11) 1,1-Dichloroethene-d2	4.021	65	103200	24.275	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 97.120%			
21) 2-Butanone-d5	7.081	46	114778	40.894	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 81.780%			
24) Chloroform-d	7.648	84	414589	23.998	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 96.000%			
26) 1,2-Dichloroethane-d4	8.307	65	237149	24.276	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 97.120%			
32) Benzene-d6	8.276	84	857818	24.778	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 99.120%			
36) 1,2-Dichloropropane-d6	9.276	67	276802	24.989	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 99.960%			
41) Toluene-d8	10.325	98	739196	23.944	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 95.760%			
43) trans-1,3-Dichloroprop...	10.575	79	101553	22.618	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 90.480%			
47) 2-Hexanone-d5	10.922	63	75446	39.944	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 79.880%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	192230	22.769	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 91.080%			
66) 1,2-Dichlorobenzene-d4	13.849	152	197115	25.195	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 100.760%			
Target Compounds						Qvalue
68) 1,2-Dibromo-3-chloropr...	14.617	75	1041	0.885	ug/L	# 11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
Data File : VW025872.D
Acq On : 08 May 2023 10:26
Operator : SY/MD
Sample : VW0508SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 09 02:56:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 05 23:47:36 2023
Response via : Initial Calibration

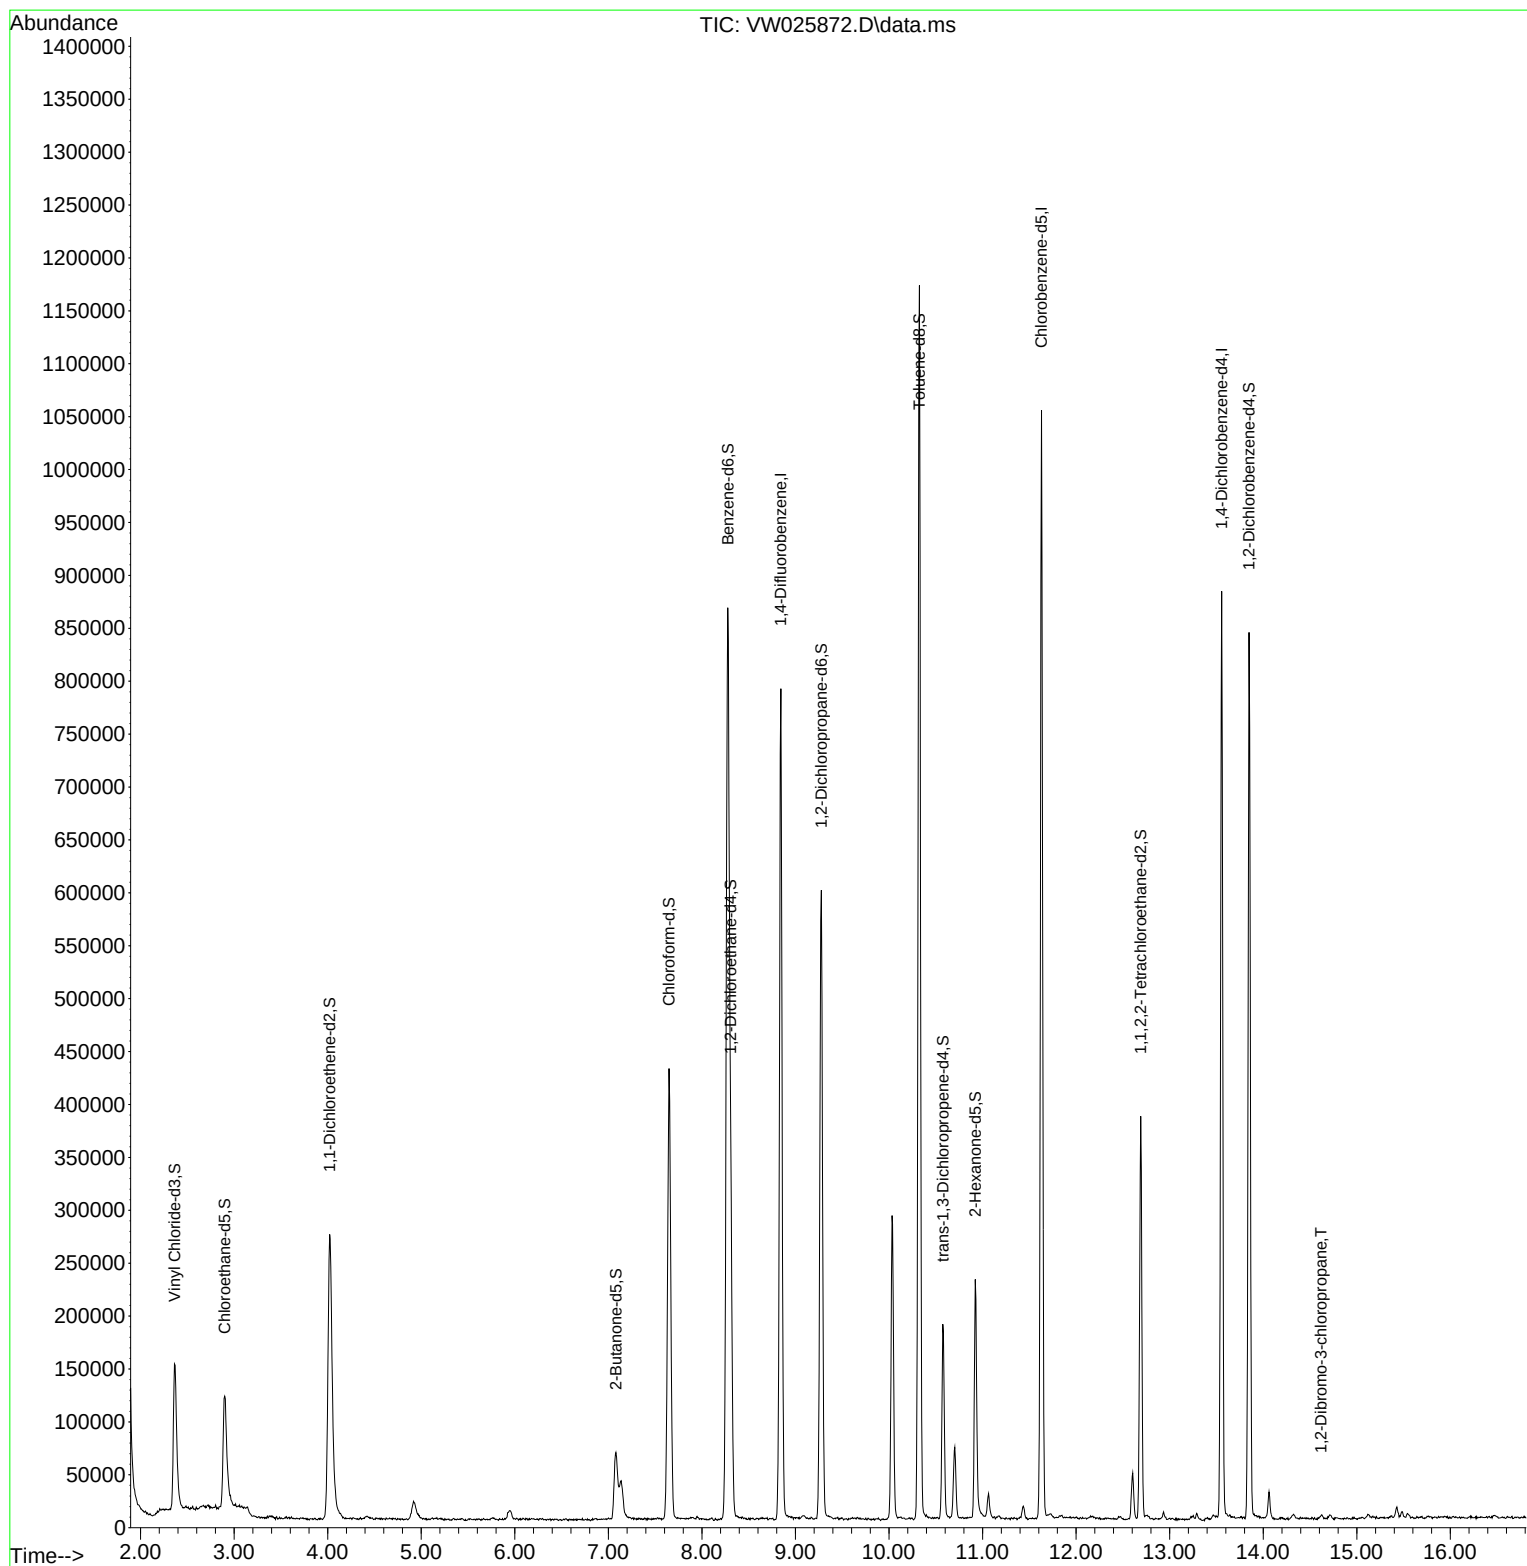

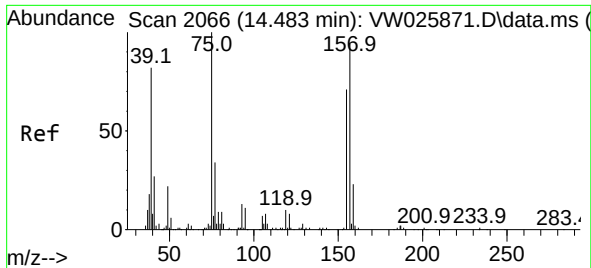

#68
 1,2-Dibromo-3-chloropropane
 Concen: 0.885 ug/L
 RT: 14.617 min Scan# 2066
 Delta R.T. 0.134 min
 Lab File: VW025872.D
 Acq: 08 May 2023 10:26

Instrument :
 MSVOA_W
 ClientSampleId :

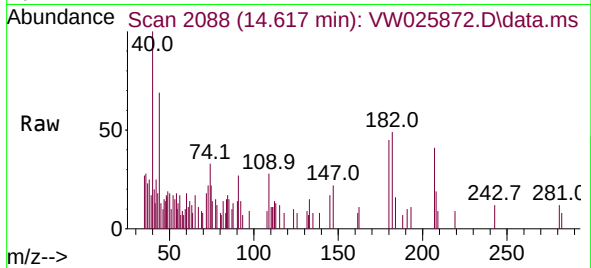

Tgt Ion: 75 Resp: 1041
 Ion Ratio Lower Upper
 75 100
 155 0.0 56.3 84.5#
 157 0.0 66.3 99.5#

