


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
Data File : VW025881.D
Acq On : 08 May 2023 15:39
Operator : SY/MD
Sample : 02592-32
Misc : 4.79g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JREG1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2023
Supervised By :Mahesh Dadoda 05/09/2023

Quant Time: May 09 02:58:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 05 23:47:36 2023
Response via : Initial Calibration

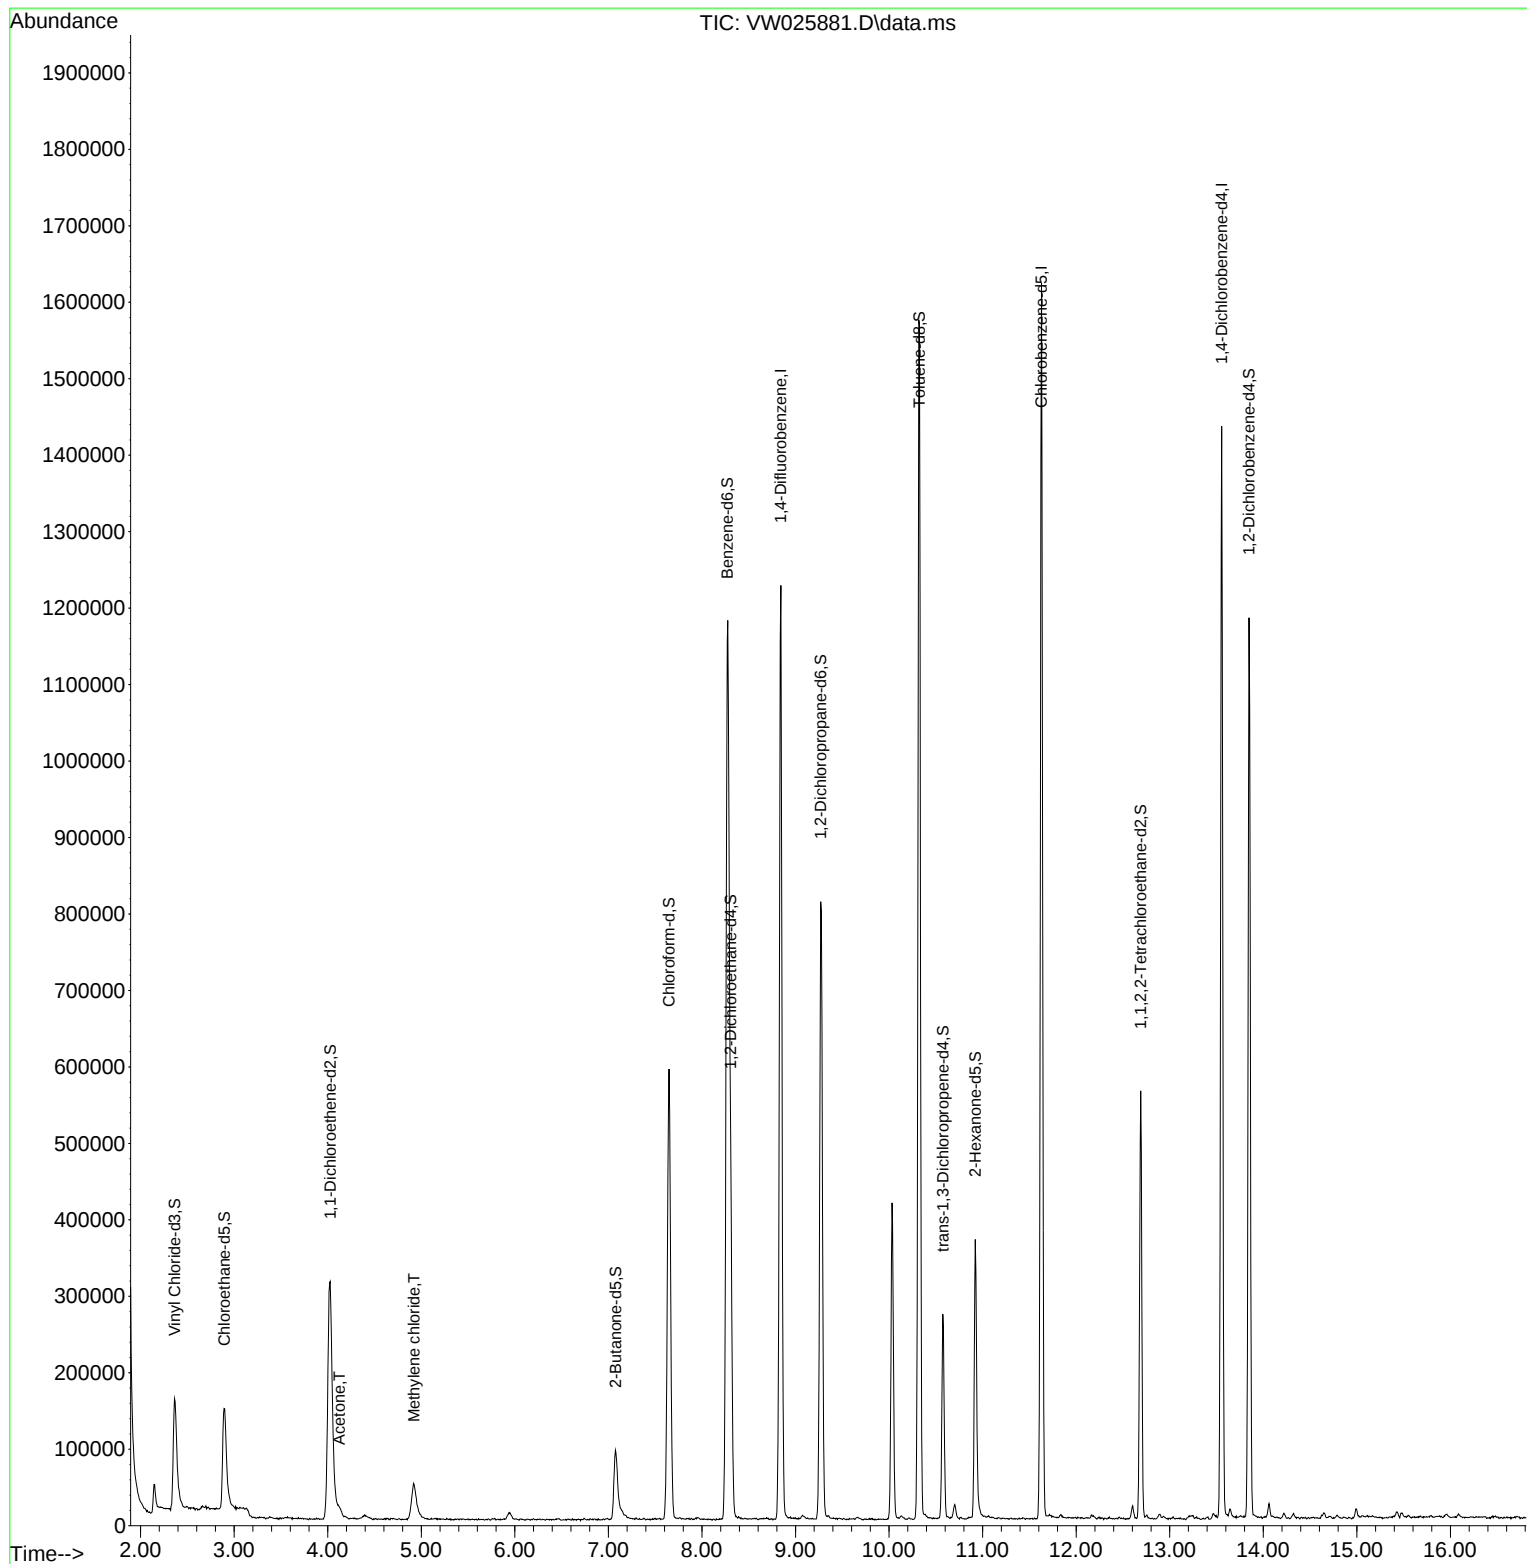




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
 Data File : VW025881.D
 Acq On : 08 May 2023 15:39
 Operator : SY/MD
 Sample : 02592-32
 Misc : 4.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JREG1

Manual IntegrationsAPPROVED

Quant Time: May 09 02:58:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/09/2023
 Supervised By :Mahesh Dadoda 05/09/2023

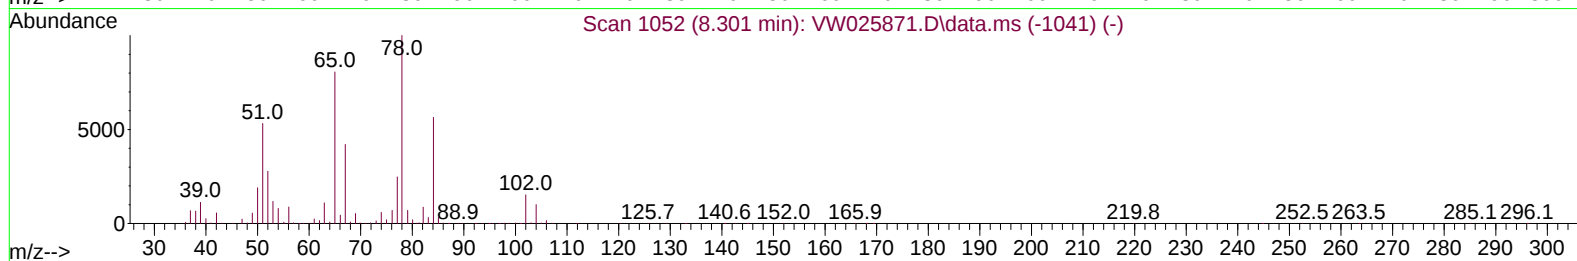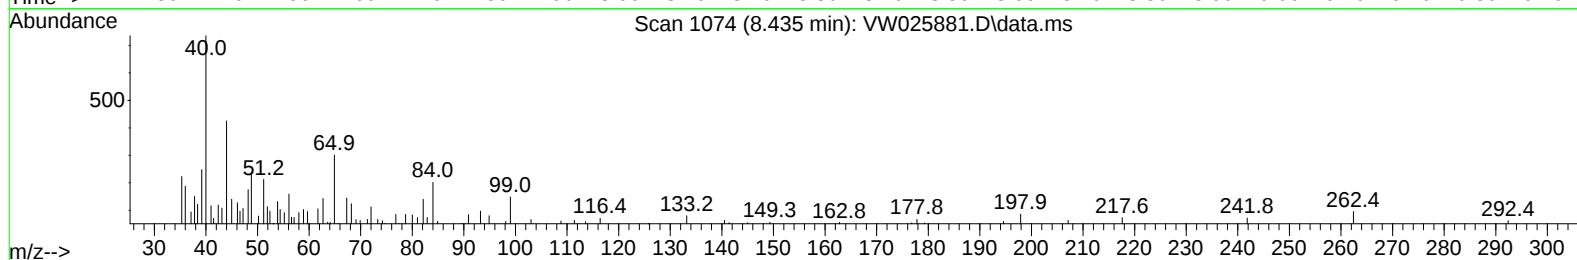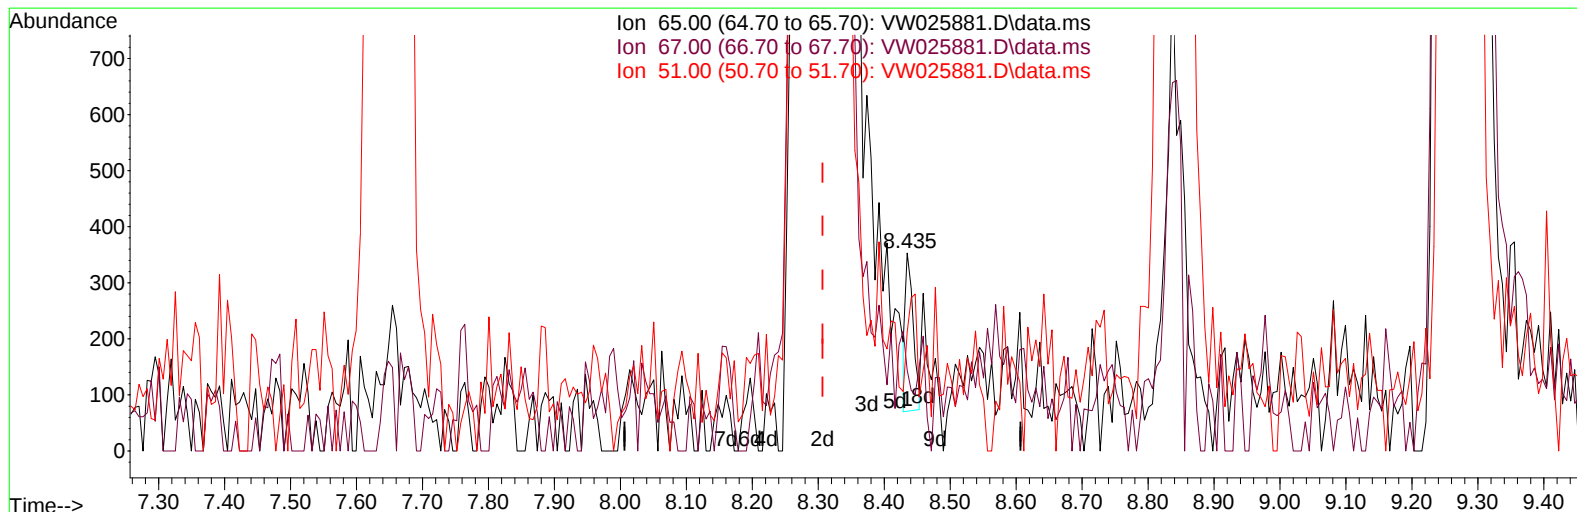

TIC: VW025881.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.435min (+ 0.128) 0.02 ug/L

response 231

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	59.74
51.00	112.30	123.81
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
 Data File : VW025881.D
 Acq On : 08 May 2023 15:39
 Operator : SY/MD
 Sample : 02592-32
 Misc : 4.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JREG1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2023
 Supervised By :Mahesh Dadoda 05/09/2023

Quant Time: May 09 02:58:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

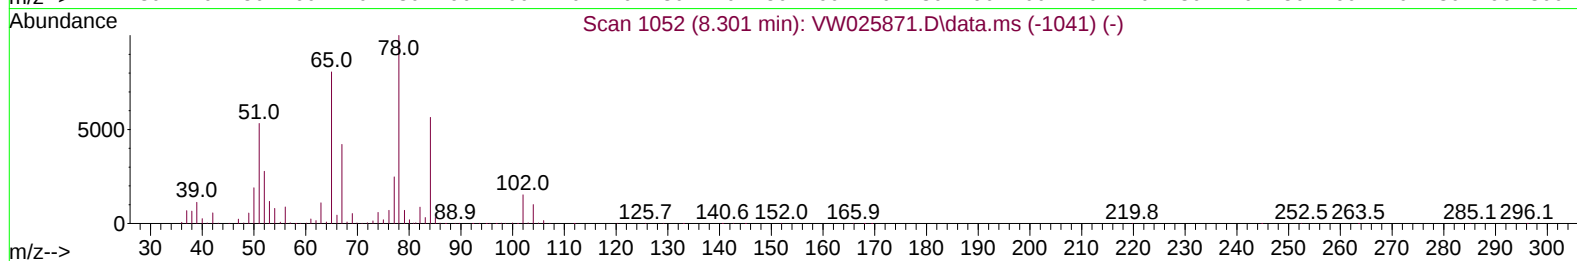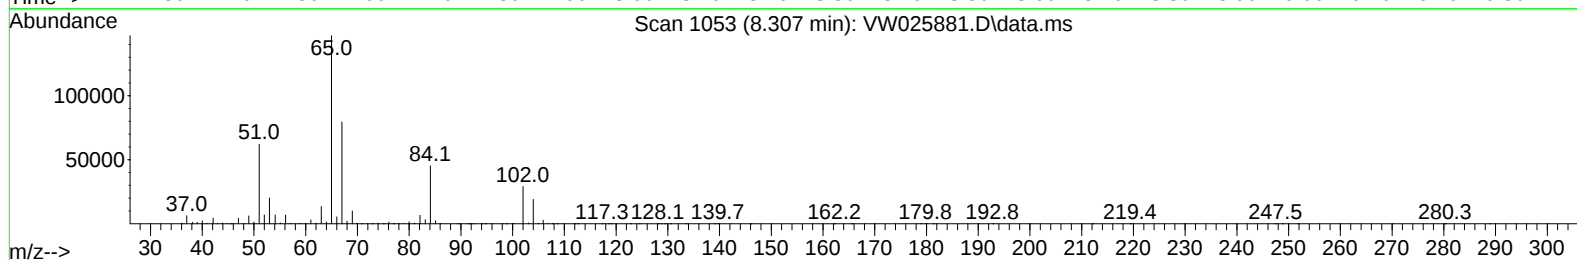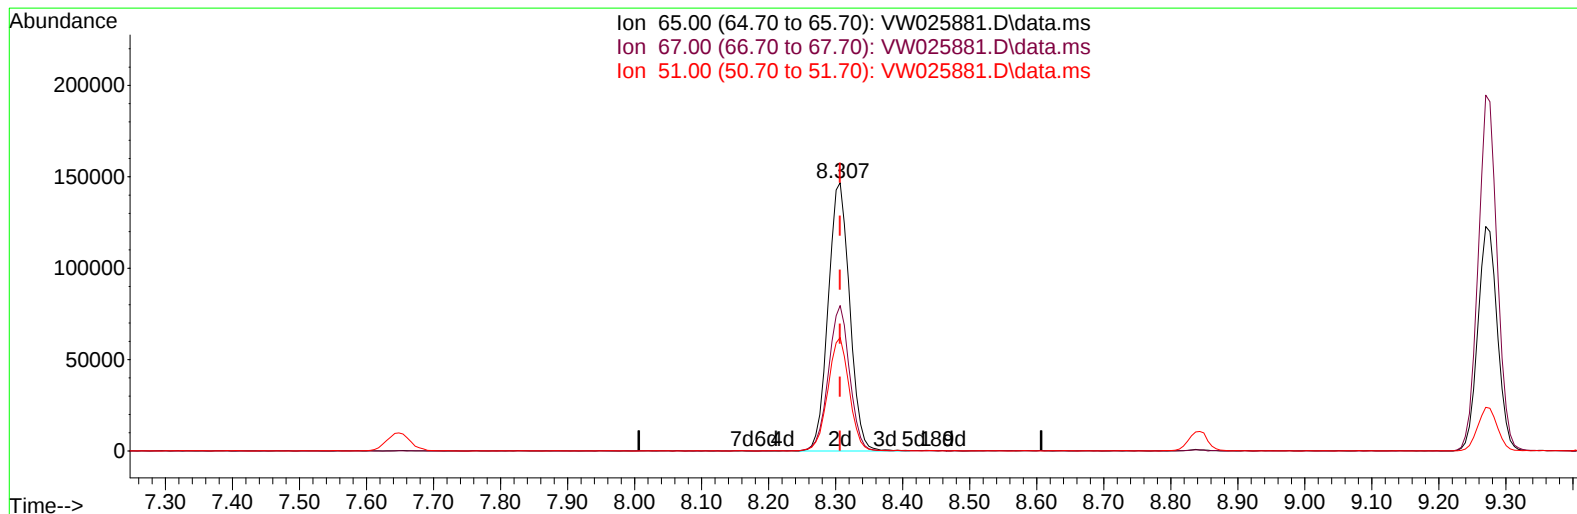

TIC: VW025881.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 21.23 ug/L m

response 326804

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.04#
51.00	112.30	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
 Data File : VW025881.D
 Acq On : 08 May 2023 15:39
 Operator : SY/MD
 Sample : 02592-32
 Misc : 4.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JREG1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2023
 Supervised By :Mahesh Dadoda 05/09/2023

Quant Time: May 09 02:58:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	944196	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	815213	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	337328	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	260256	19.451	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.800%		
7) Chloroethane-d5	2.893	69	216347	21.810	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.240%		
11) 1,1-Dichloroethene-d2	4.027	65	131850	19.680	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	78.720%		
21) 2-Butanone-d5	7.075	46	160394	36.262	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	72.520%		
24) Chloroform-d	7.648	84	581342	21.352	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.400%		
26) 1,2-Dichloroethane-d4	8.307	65	326804m	21.227	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	84.920%		
32) Benzene-d6	8.270	84	1179115	22.136	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.560%		
36) 1,2-Dichloropropane-d6	9.270	67	384660	22.570	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	90.280%		
41) Toluene-d8	10.325	98	1018327	21.439	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.760%		
43) trans-1,3-Dichloroprop...	10.575	79	141960	20.549	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.200%		
47) 2-Hexanone-d5	10.922	63	120249	41.377	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	82.760%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	283482	21.823	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	87.280%		
66) 1,2-Dichlorobenzene-d4	13.848	152	277747	22.587	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.360%		
Target Compounds					Qvalue	
13) Acetone	4.125	43	19796	5.047	ug/L	94
16) Methylene chloride	4.923	84	40957	2.103	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed