

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
 Data File : VW025873.D
 Acq On : 08 May 2023 12:28
 Operator : SY/MD
 Sample : 02592-23
 Misc : 3.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JREJ8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2023
 Supervised By :Mahesh Dadoda 05/09/2023

Quant Time: May 09 02:56:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	923453	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	710502	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	228834	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	265053	20.255	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.000%		
7) Chloroethane-d5	2.899	69	216622	22.329	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.320%		
11) 1,1-Dichloroethene-d2	4.021	65	129134	19.707	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	78.840%		
21) 2-Butanone-d5	7.081	46	129315	29.892	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	59.780%		
24) Chloroform-d	7.648	84	514672	19.328	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	77.320%		
26) 1,2-Dichloroethane-d4	8.301	65	291238m	19.342	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	77.360%		
32) Benzene-d6	8.270	84	1058082	22.791	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	91.160%		
36) 1,2-Dichloropropane-d6	9.270	67	338482	22.787	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.160%		
41) Toluene-d8	10.318	98	877332	21.192	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.760%		
43) trans-1,3-Dichloroprop...	10.575	79	115951	19.257	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.040%		
47) 2-Hexanone-d5	10.922	63	89546	35.353	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	70.700%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	196909	17.392	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	69.560%		
66) 1,2-Dichlorobenzene-d4	13.854	152	172294	20.654	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.600%		
Target Compounds					Qvalue	
13) Acetone	4.143	43	40646	10.596	ug/L	100
16) Methylene chloride	4.917	84	46061	2.419	ug/L	89
42) Toluene	10.386	91	110672	2.203	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
Data File : VW025873.D
Acq On : 08 May 2023 12:28
Operator : SY/MD
Sample : 02592-23
Misc : 3.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
JREJ8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2023
Supervised By :Mahesh Dadoda 05/09/2023


Quant Time: May 09 02:56:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 05 23:47:36 2023
Response via : Initial Calibration

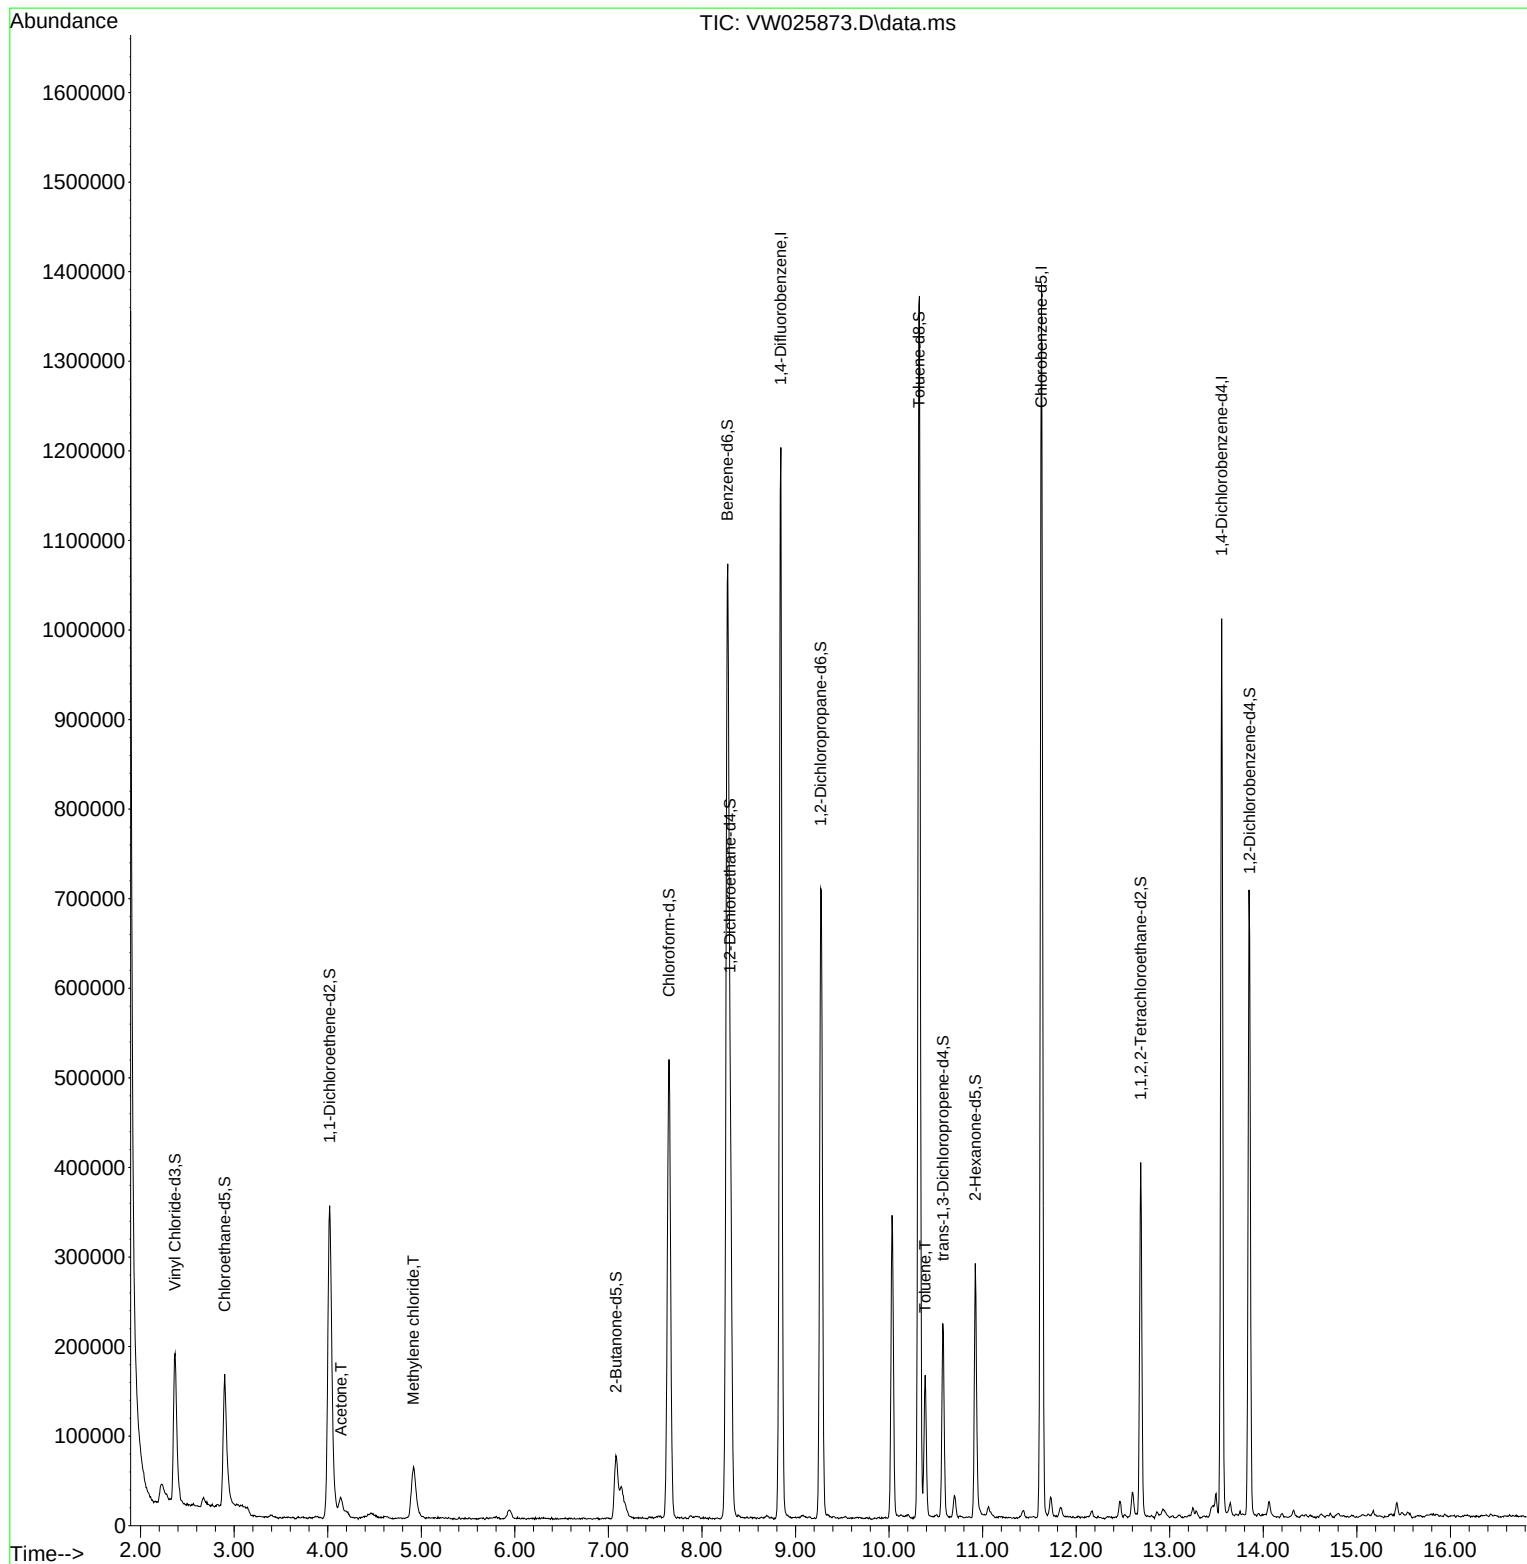

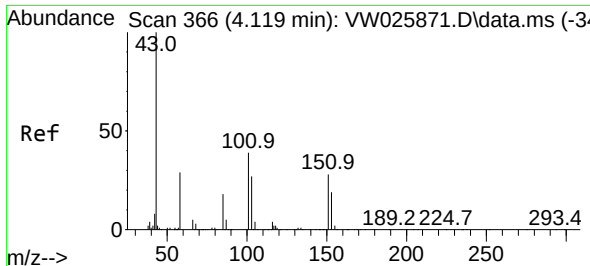

#13
Acetone
Concen: 10.596 ug/L
RT: 4.143 min Scan# 31
Delta R.T. 0.012 min
Lab File: VW025873.D
Acq: 08 May 2023 12:28




Instrument :
MSVOA_W
ClientSampleId :
JREJ8

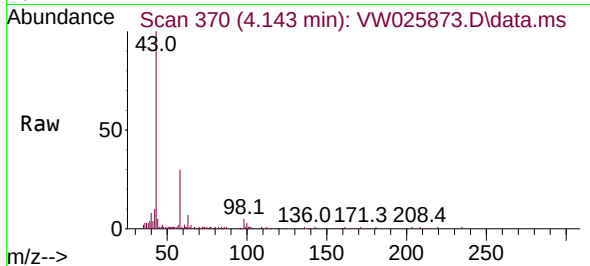

Tgt Ion: 43 Resp: 40640
Ion Ratio Lower Upper
43 100
58 29.3 0.0 58.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/09/2023
Supervised By :Mahesh Dadoda 05/09/2023

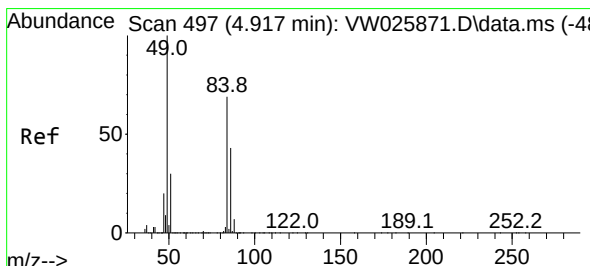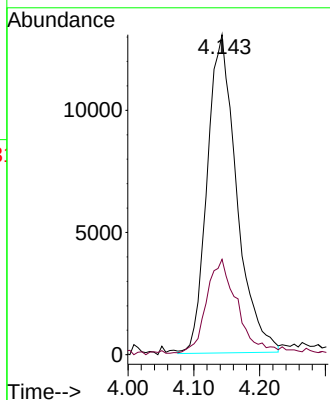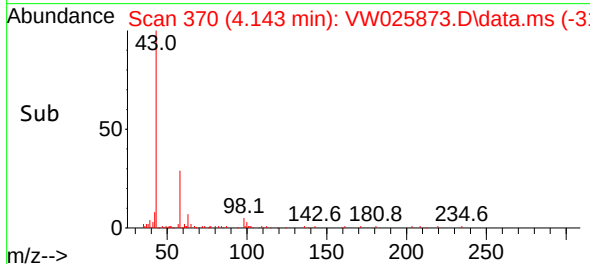

#16
Methylene chloride
Concen: 2.419 ug/L
RT: 4.917 min Scan# 497
Delta R.T. 0.006 min
Lab File: VW025873.D
Acq: 08 May 2023 12:28


Tgt Ion: 84 Resp: 46061
Ion Ratio Lower Upper
84 100
86 63.6 41.7 77.5
49 153.1 95.3 177.1

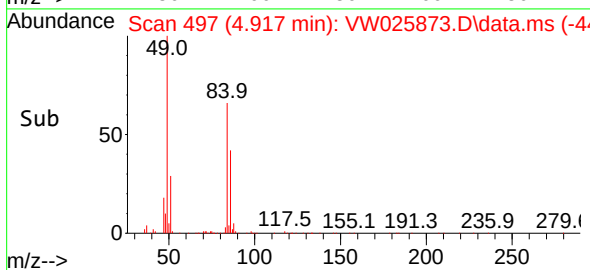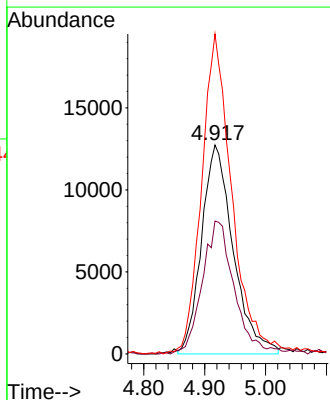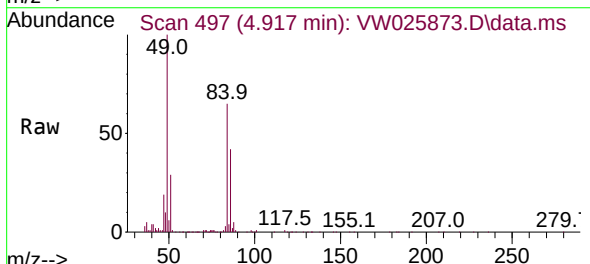

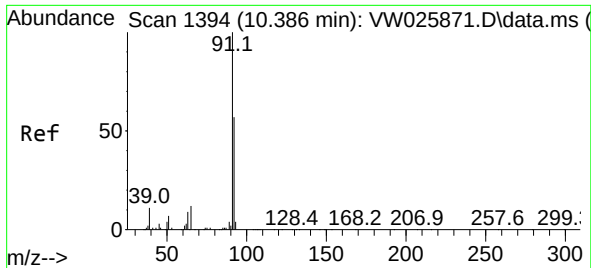

#42
Toluene
Concen: 2.203 ug/L
RT: 10.386 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW025873.D
Acq: 08 May 2023 12:28

Instrument :
MSVOA_W
ClientSampleId :
JREJ8

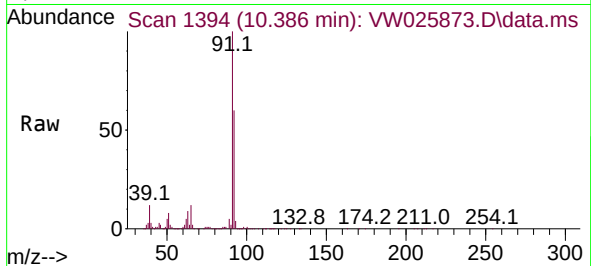

Tgt Ion: 91 Resp: 110672
Ion Ratio Lower Upper
91 100
92 59.6 40.2 74.6

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2023
Supervised By :Mahesh Dadoda 05/09/2023

