

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
 Data File : VW025887.D
 Acq On : 08 May 2023 18:04
 Operator : SY/MD
 Sample : 02612-19
 Misc : 3.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JREA3

Quant Time: May 09 02:59:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	856963	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	654090	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	189742	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	257393	21.196	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.800%
7) Chloroethane-d5	2.893	69	215399	23.925	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.720%
11) 1,1-Dichloroethene-d2	4.021	65	129394	21.279	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.120%
21) 2-Butanone-d5	7.075	46	156046	38.870	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.740%
24) Chloroform-d	7.648	84	526389	21.302	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.200%
26) 1,2-Dichloroethane-d4	8.307	65	305059	21.832	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.320%
32) Benzene-d6	8.270	84	1101550	25.774	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.080%
36) 1,2-Dichloropropane-d6	9.270	67	359777	26.310	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.240%
41) Toluene-d8	10.325	98	917590	24.076	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.320%
43) trans-1,3-Dichloroprop...	10.575	79	112653	20.323	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.280%
47) 2-Hexanone-d5	10.922	63	105816	45.379	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.760%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	222102	21.309	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.240%
66) 1,2-Dichlorobenzene-d4	13.848	152	161937	23.412	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.640%
Target Compounds					Qvalue	
13) Acetone	4.125	43	36148	10.155	ug/L	100
16) Methylene chloride	4.923	84	34136	1.932	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050823\
Data File : VW025887.D
Acq On : 08 May 2023 18:04
Operator : SY/MD
Sample : 02612-19
Misc : 3.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JREA3

Quant Time: May 09 02:59:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 05 23:47:36 2023
Response via : Initial Calibration




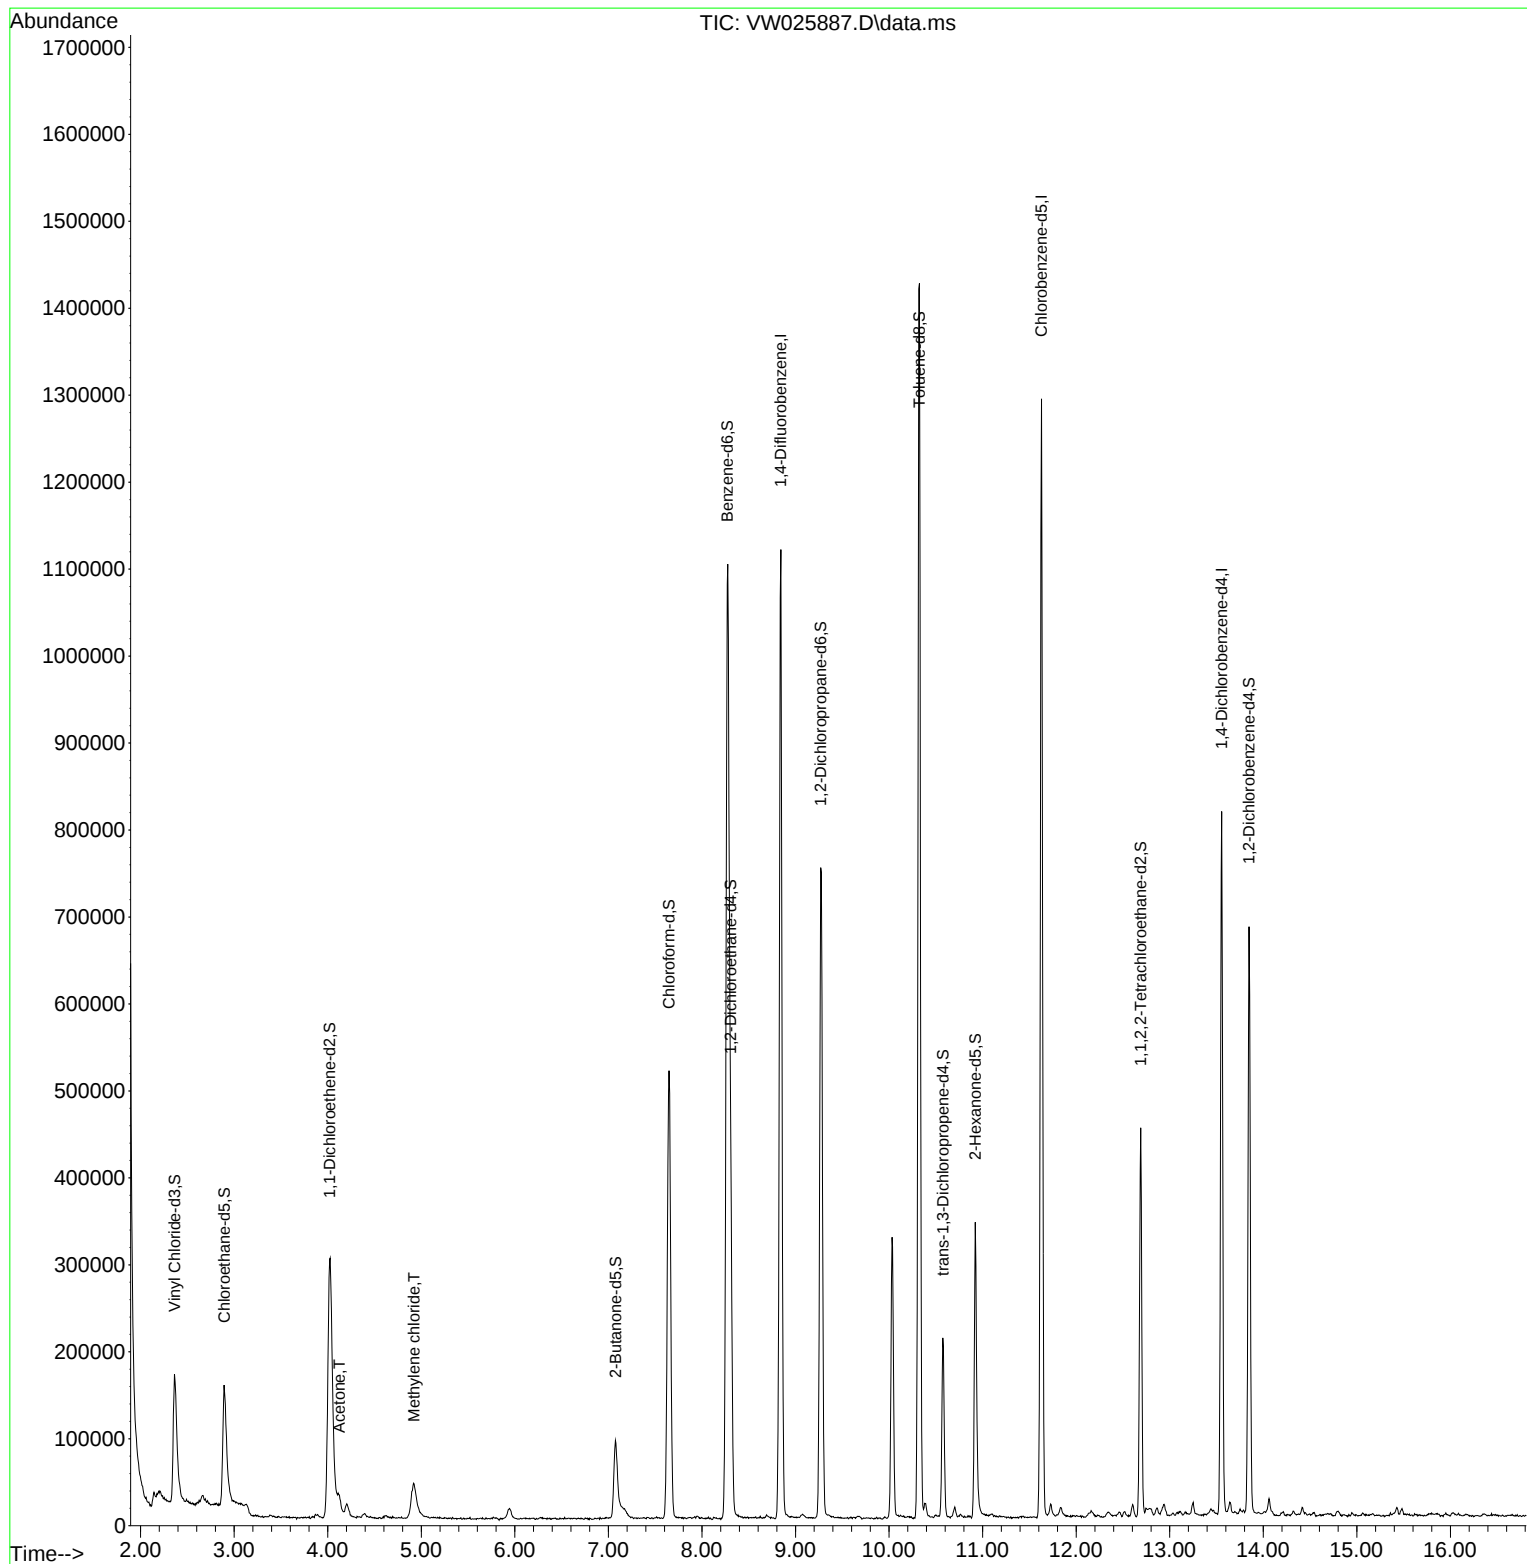


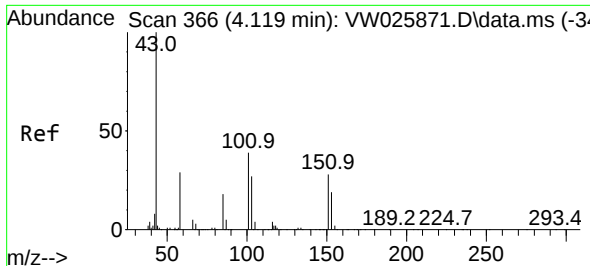

#13
Acetone
Concen: 10.155 ug/L
RT: 4.125 min Scan# 367
Delta R.T. -0.006 min
Lab File: VW025887.D
Acq: 08 May 2023 18:04

Instrument :
MSVOA_W
ClientSampleId :
JREA3

Tgt Ion: 43 Resp: 36148
Ion Ratio Lower Upper
43 100
58 29.3 0.0 58.2

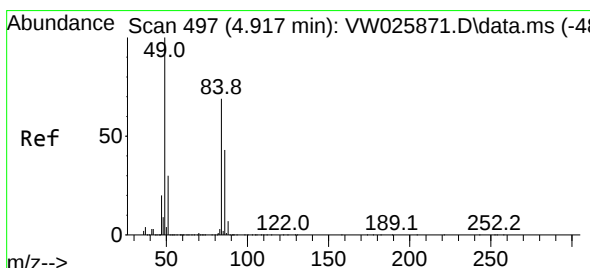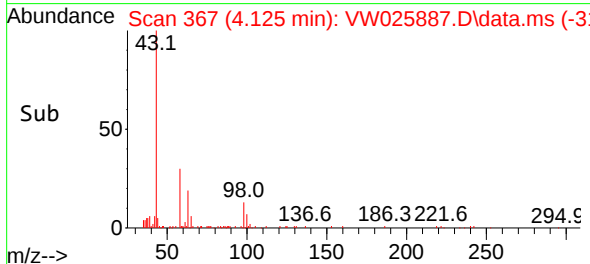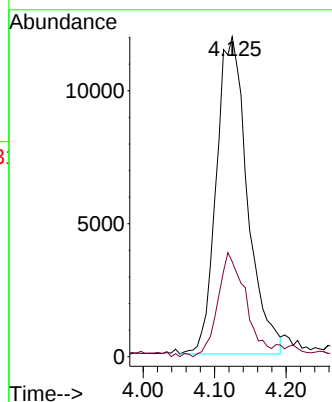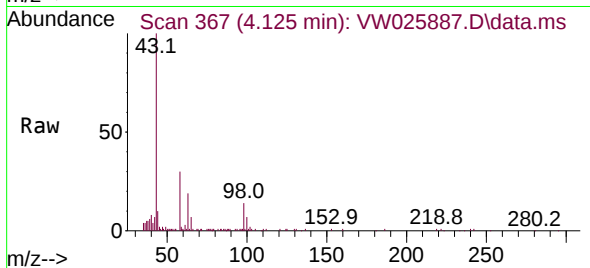

#16
Methylene chloride
Concen: 1.932 ug/L
RT: 4.923 min Scan# 498
Delta R.T. 0.012 min
Lab File: VW025887.D
Acq: 08 May 2023 18:04

Tgt Ion: 84 Resp: 34136
Ion Ratio Lower Upper
84 100
86 59.1 41.7 77.5
49 140.0 95.3 177.1

