

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022922.D
 Acq On : 09 May 2022 12:04
 Operator : SY/VA
 Sample : N2638-24
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: May 09 22:56:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	338018	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	328205	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	159903	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	115054	16.590	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.360%
7) Chloroethane-d5	2.885	69	87860	19.474	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.880%
11) 1,1-Dichloroethene-d2	4.013	63	123515	13.784	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.120%
21) 2-Butanone-d5	7.080	46	54105	41.034	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.060%
24) Chloroform-d	7.647	84	201559	20.353	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.400%
26) 1,2-Dichloroethane-d4	8.305	65	109352	20.133	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.520%
32) Benzene-d6	8.275	84	389992	20.615	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.480%
36) 1,2-Dichloropropane-d6	9.274	67	112086	21.093	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.360%
41) Toluene-d8	10.323	98	364968	19.972	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.880%
43) trans-1,3-Dichloroprop...	10.579	79	45124	18.442	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.760%
47) 2-Hexanone-d5	10.927	63	41553	40.962	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.920%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	100940	20.380	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	122133	21.850	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.400%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4105	0.566	ug/L	# 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
Data File : VW022922.D
Acq On : 09 May 2022 12:04
Operator : SY/VA
Sample : N2638-24
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: May 09 22:56:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 09 22:55:00 2022
Response via : Initial Calibration

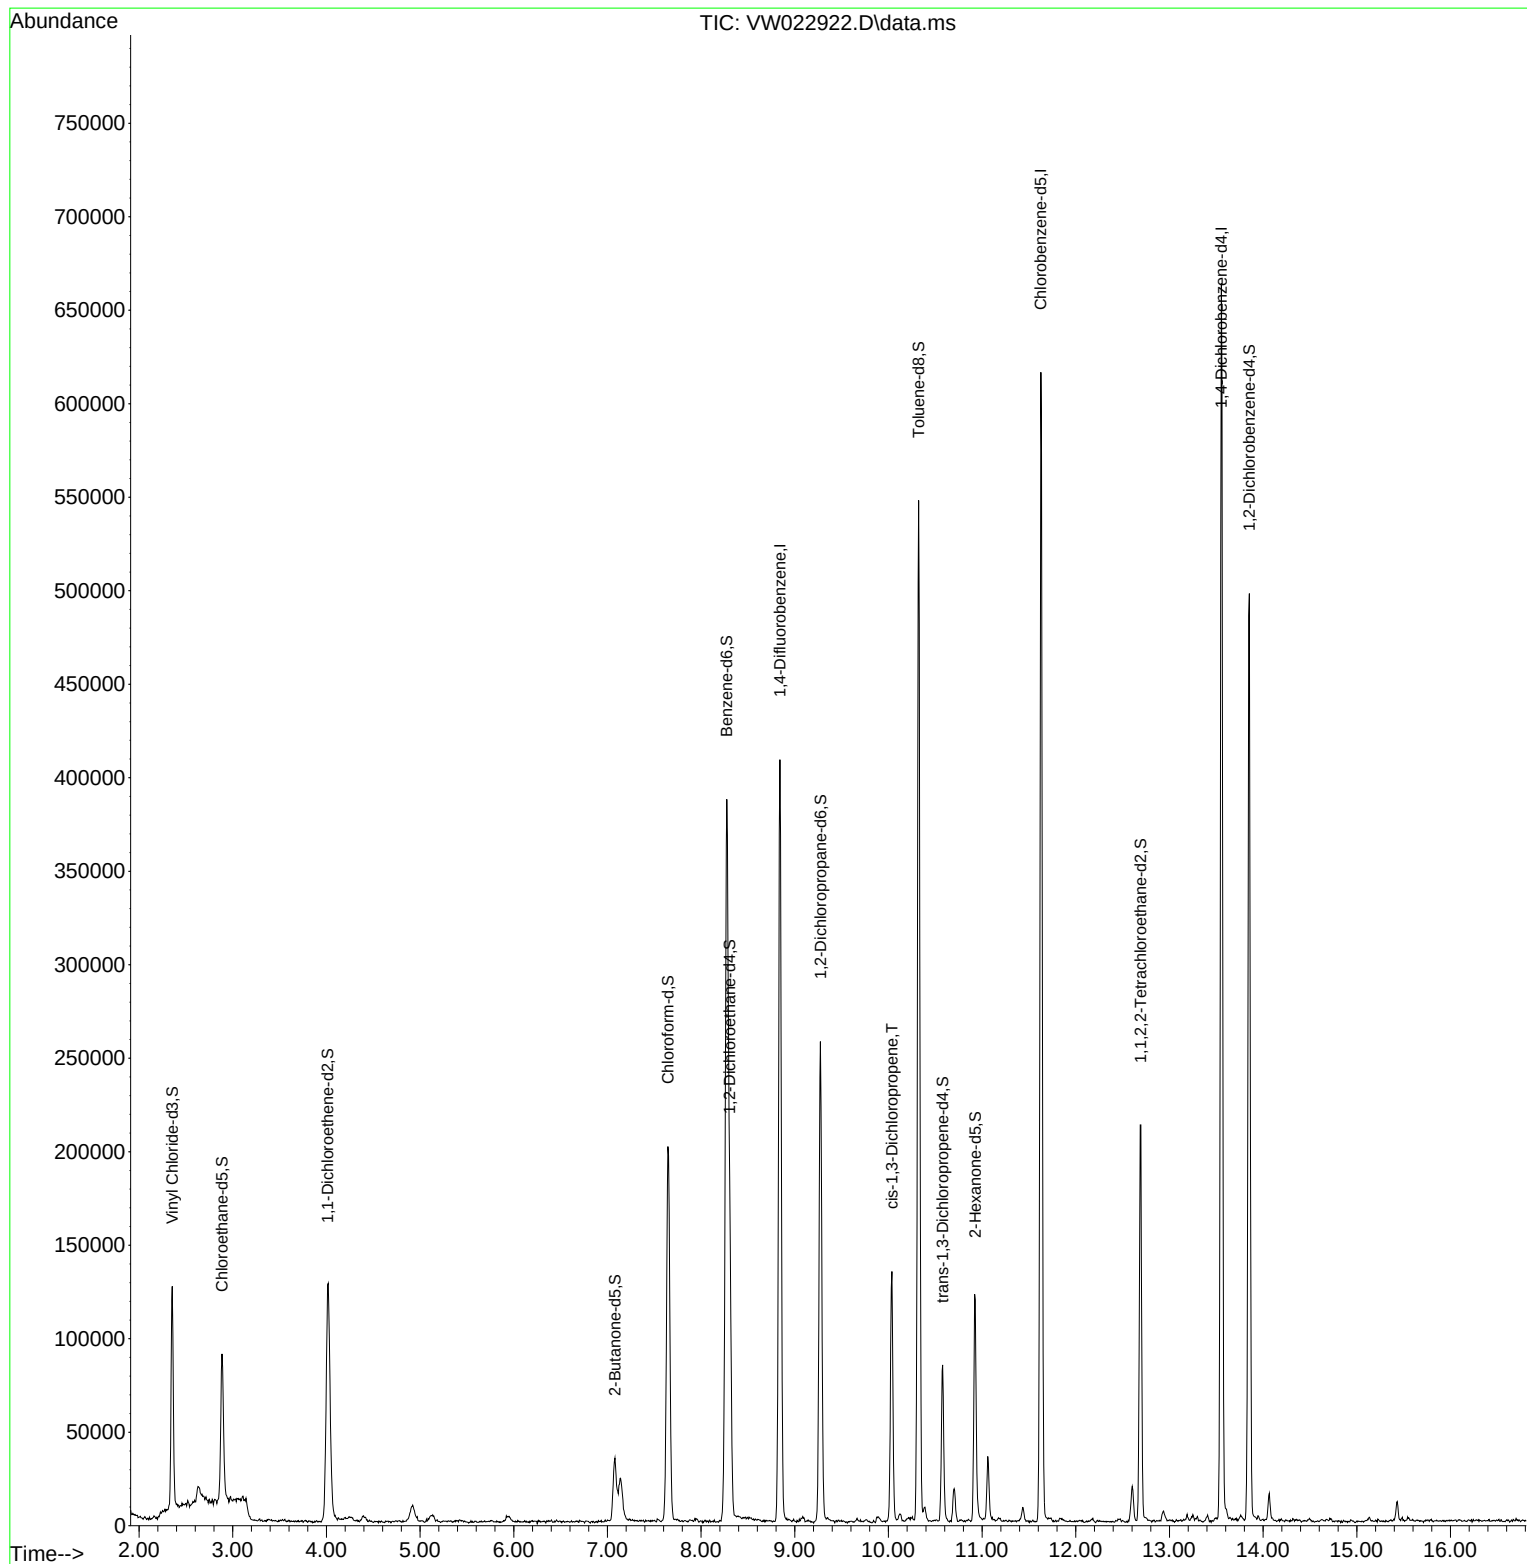

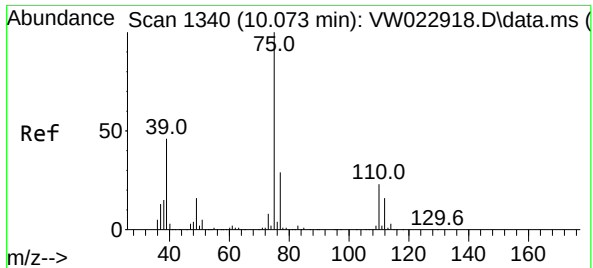

#39
 cis-1,3-Dichloropropene
 Concen: 0.566 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022922.D
 Acq: 09 May 2022 12:04

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Tgt Ion: 75 Resp: 4105
 Ion Ratio Lower Upper
 75 100
 77 52.9 22.1 41.1#

