

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022923.D
 Acq On : 09 May 2022 12:28
 Operator : SY/VA
 Sample : N2713-12
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSL3

Quant Time: May 09 22:56:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	389169	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	379137	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	186802	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	120145	15.048	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.200%
7) Chloroethane-d5	2.885	69	92081	17.727	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.920%
11) 1,1-Dichloroethene-d2	4.019	63	129976	12.599	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.400%
21) 2-Butanone-d5	7.074	46	69284	45.639	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.280%
24) Chloroform-d	7.647	84	233586	20.487	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.960%
26) 1,2-Dichloroethane-d4	8.305	65	134178	21.457	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.840%
32) Benzene-d6	8.275	84	434310	19.874	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.480%
36) 1,2-Dichloropropane-d6	9.274	67	132151	21.528	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.120%
41) Toluene-d8	10.323	98	402770	19.079	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.320%
43) trans-1,3-Dichloroprop...	10.579	79	55819	19.749	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.000%
47) 2-Hexanone-d5	10.920	63	55990	47.779	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.560%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	130030	22.726	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.920%
66) 1,2-Dichlorobenzene-d4	13.853	152	149639	22.916	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.680%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4899	0.585	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
Data File : VW022923.D
Acq On : 09 May 2022 12:28
Operator : SY/VA
Sample : N2713-12
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSL3

Quant Time: May 09 22:56:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 09 22:55:00 2022
Response via : Initial Calibration

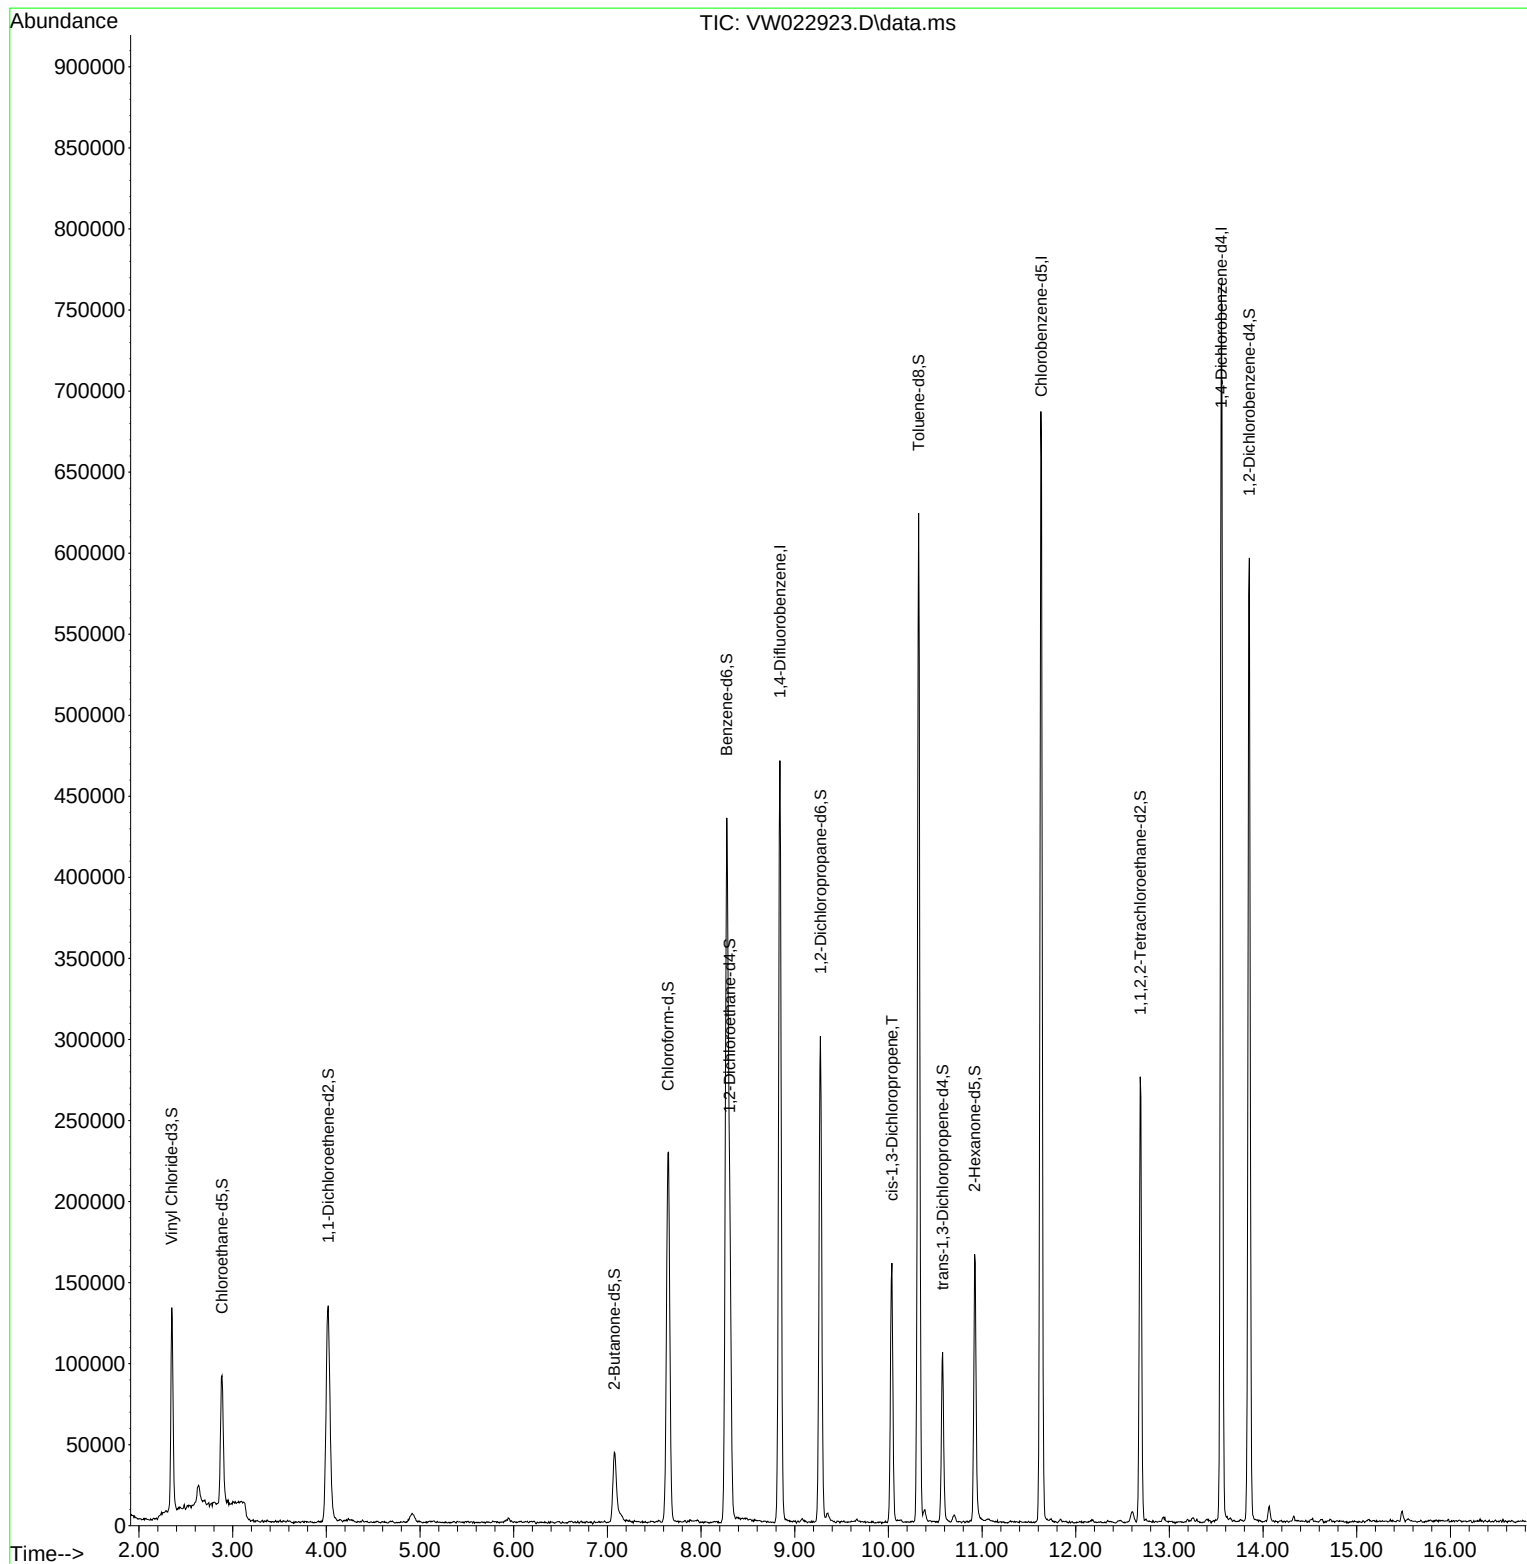

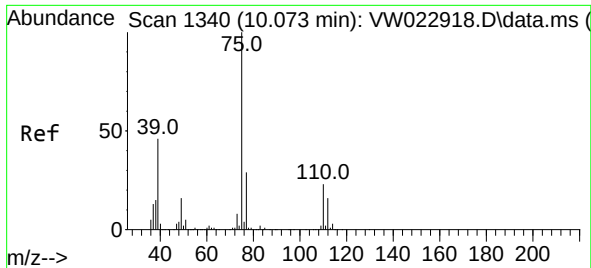

#39
 cis-1,3-Dichloropropene
 Concen: 0.585 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022923.D
 Acq: 09 May 2022 12:28

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSL3

Tgt Ion: 75 Resp: 4899
 Ion Ratio Lower Upper
 75 100
 77 38.1 22.1 41.1

