

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022928.D
 Acq On : 09 May 2022 14:28
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK452

Quant Time: May 09 22:58:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	314923	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	305980	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	152117	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	115798	17.922	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.680%
7) Chloroethane-d5	2.885	69	89183	21.217	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.880%
11) 1,1-Dichloroethene-d2	4.019	63	126514	15.154	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.600%
21) 2-Butanone-d5	7.074	46	55263	44.985	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.980%
24) Chloroform-d	7.653	84	214880	23.289	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.160%
26) 1,2-Dichloroethane-d4	8.409	65	129	0.025	ug/L	0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.275	84	405059	22.967	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.880%
36) 1,2-Dichloropropane-d6	9.274	67	120752	24.374	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.480%
41) Toluene-d8	10.323	98	378233	22.201	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.800%
43) trans-1,3-Dichloroprop...	10.579	79	47591	20.863	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.440%
47) 2-Hexanone-d5	10.927	63	45395	48.000	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.000%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	106116	22.981	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.920%
66) 1,2-Dichlorobenzene-d4	13.853	152	129347	24.325	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.280%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4477	0.662	ug/L #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
Data File : VW022928.D
Acq On : 09 May 2022 14:28
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK452

Quant Time: May 09 22:58:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 09 22:55:00 2022
Response via : Initial Calibration

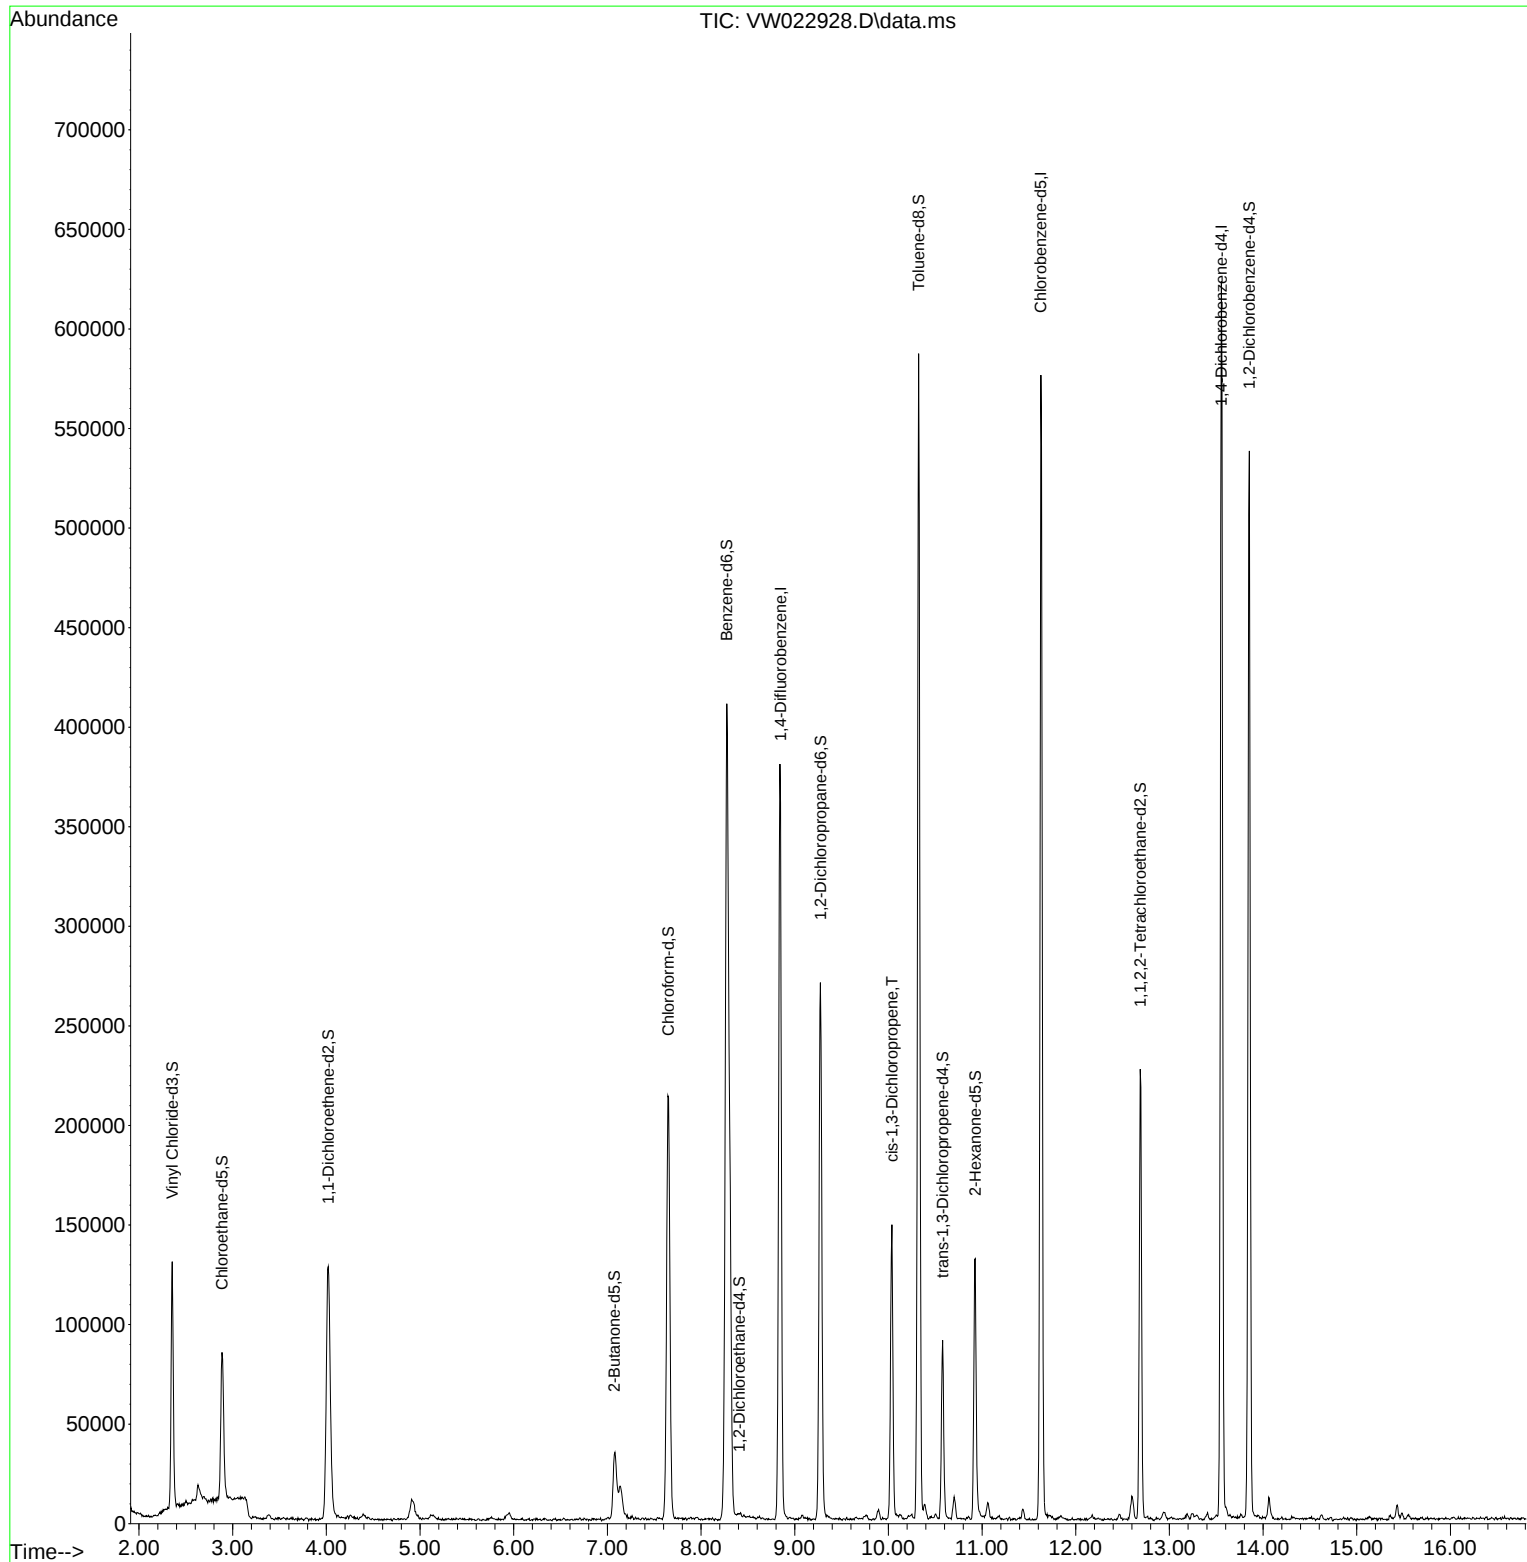

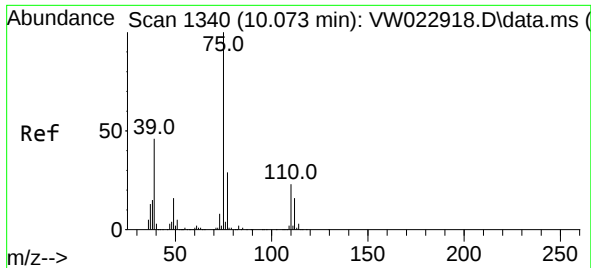

#39
 cis-1,3-Dichloropropene
 Concen: 0.662 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022928.D
 Acq: 09 May 2022 14:28

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK452

Tgt Ion: 75 Resp: 4477
 Ion Ratio Lower Upper
 75 100
 77 43.7 22.1 41.1#

