

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022931.D
 Acq On : 09 May 2022 15:40
 Operator : SY/VA
 Sample : N2713-15
 Misc : 5.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSL4

Quant Time: May 09 22:58:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	349685	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	350083	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	171532	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	97623	13.607	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.440%
7) Chloroethane-d5	2.891	69	76479	16.386	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.560%
11) 1,1-Dichloroethene-d2	4.013	63	104930	11.319	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	45.280%
21) 2-Butanone-d5	7.074	46	49219	36.083	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.160%
24) Chloroform-d	7.647	84	189525	18.499	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.000%
26) 1,2-Dichloroethane-d4	8.305	65	104739	18.640	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	74.560%
32) Benzene-d6	8.275	84	350651	17.377	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	69.520%
36) 1,2-Dichloropropane-d6	9.274	67	107143	18.902	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.600%
41) Toluene-d8	10.323	98	326870	16.769	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.080%
43) trans-1,3-Dichloroprop...	10.579	79	42430	16.257	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.040%
47) 2-Hexanone-d5	10.920	63	38823	35.879	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.760%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	98443	18.633	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	74.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	114454	19.088	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	76.360%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.043	75	4134	0.534	ug/L	88
48) 2-Hexanone	10.920	43	4445	2.115	ug/L #	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
Data File : VW022931.D
Acq On : 09 May 2022 15:40
Operator : SY/VA
Sample : N2713-15
Misc : 5.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSL4

Quant Time: May 09 22:58:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 09 22:55:00 2022
Response via : Initial Calibration

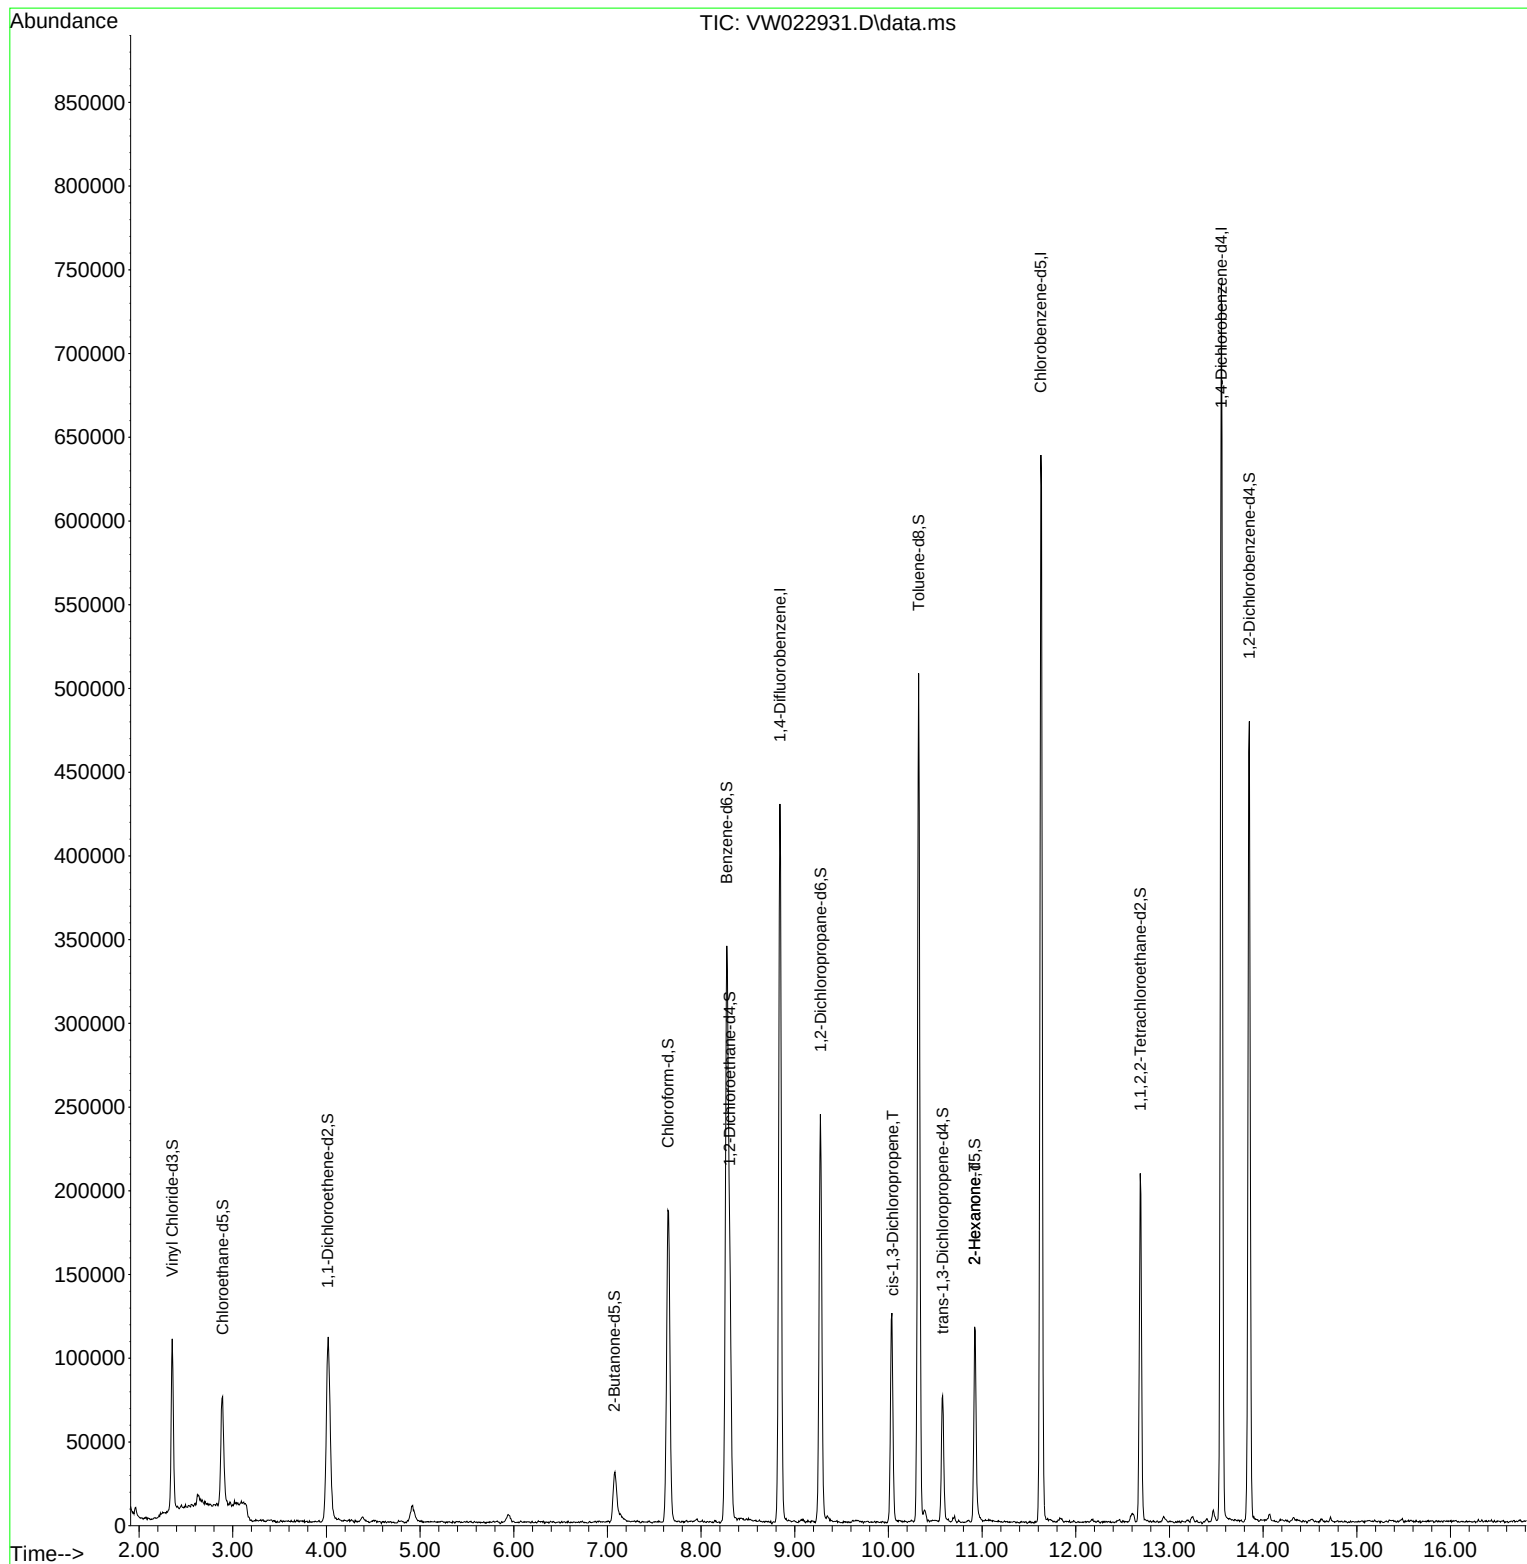

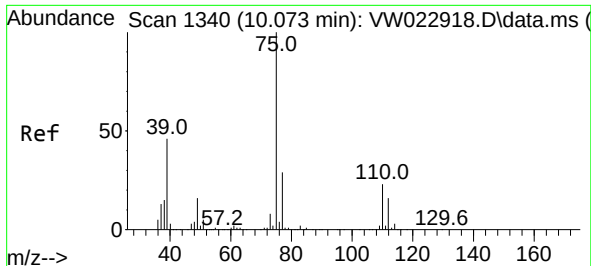

#39

cis-1,3-Dichloropropene

Concen: 0.534 ug/L

RT: 10.043 min Scan# 11

Delta R.T. -0.031 min

Lab File: VW022931.D

Acq: 09 May 2022 15:40

Instrument :

MSVOA_W

ClientSampleId :





DBSL4

Tgt Ion: 75 Resp: 4134

Ion Ratio Lower Upper

75 100

77 25.1 22.1 41.1

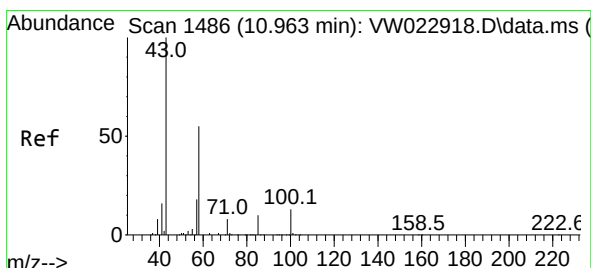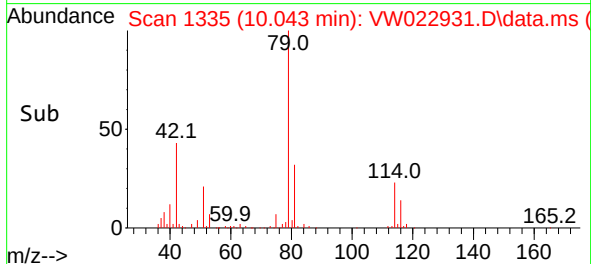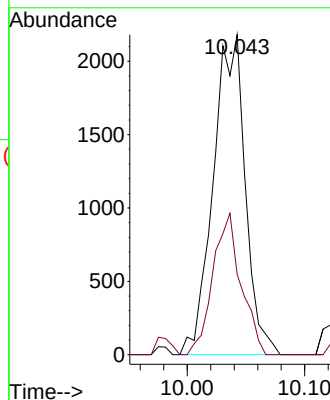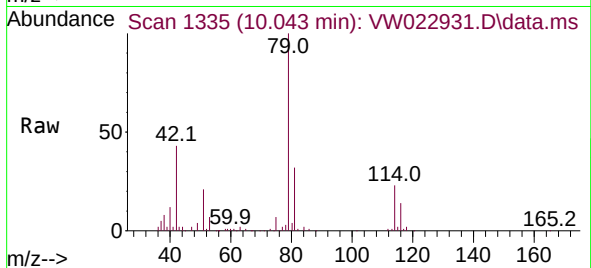

#48

2-Hexanone

Concen: 2.115 ug/L

RT: 10.920 min Scan# 1479

Delta R.T. -0.043 min

Lab File: VW022931.D

Acq: 09 May 2022 15:40

Tgt Ion: 43 Resp: 4445

Ion Ratio Lower Upper

43 100

58 0.0 45.9 68.9#

57 39.2 16.2 24.2#

100 1.7 10.7 16.1#

