




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022927.D
 Acq On : 09 May 2022 14:04
 Operator : SY/VA
 Sample : N2713-08
 Misc : 6.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSK8

Manual IntegrationsAPPROVED

Quant Time: May 09 22:57:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/10/2022

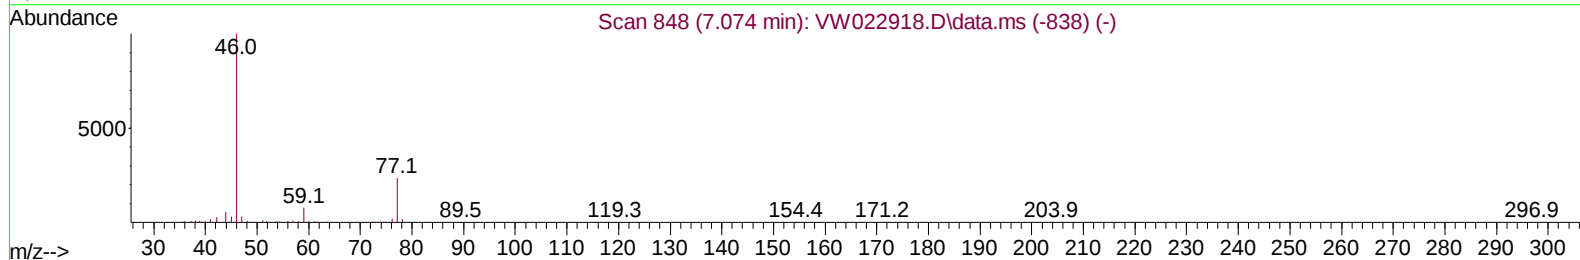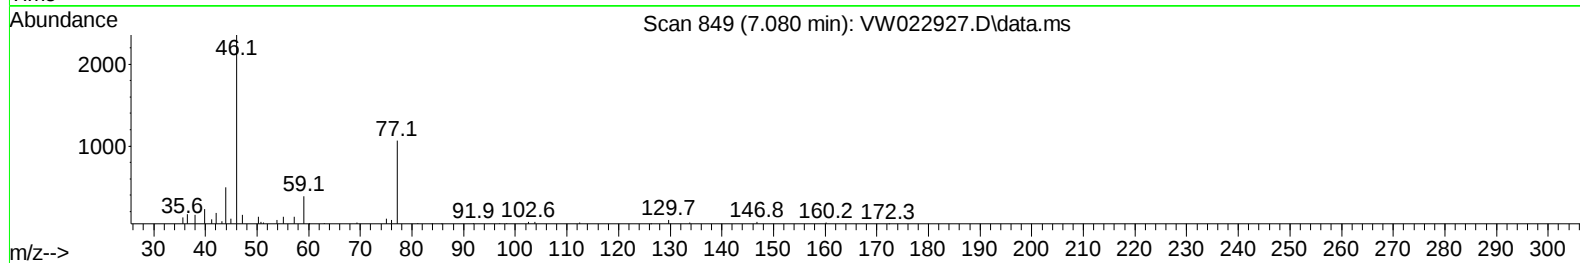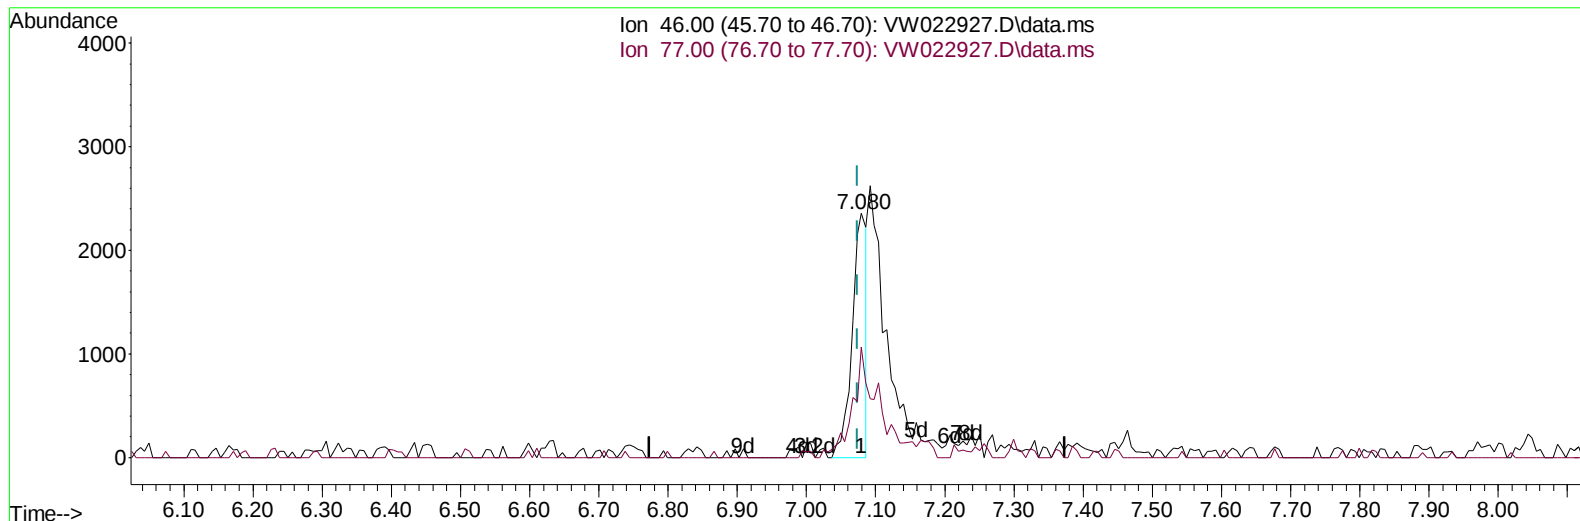

TIC: VW022927.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 35.76 ug/L

response 3431

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	46.40#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
Data File : VW022927.D
Acq On : 09 May 2022 14:04
Operator : SY/VA
Sample : N2713-08
Misc : 6.14g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSK8

Manual IntegrationsAPPROVED

Quant Time: May 09 22:57:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 09 22:55:00 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/10/2022

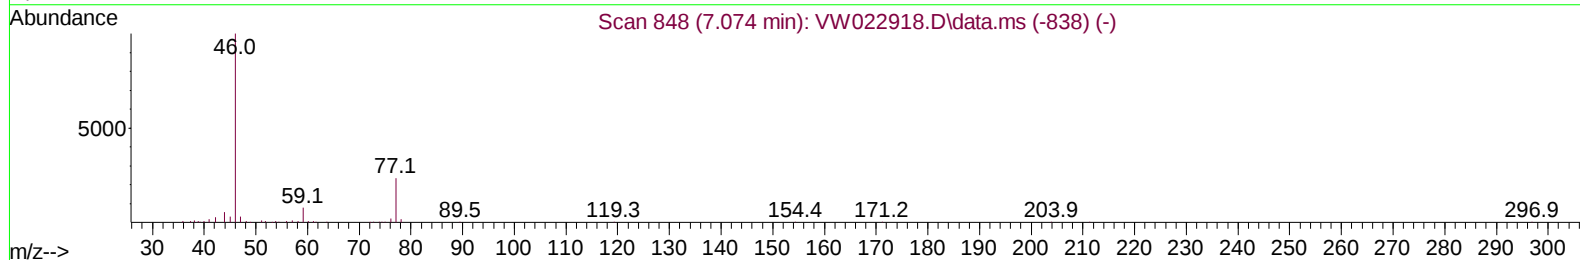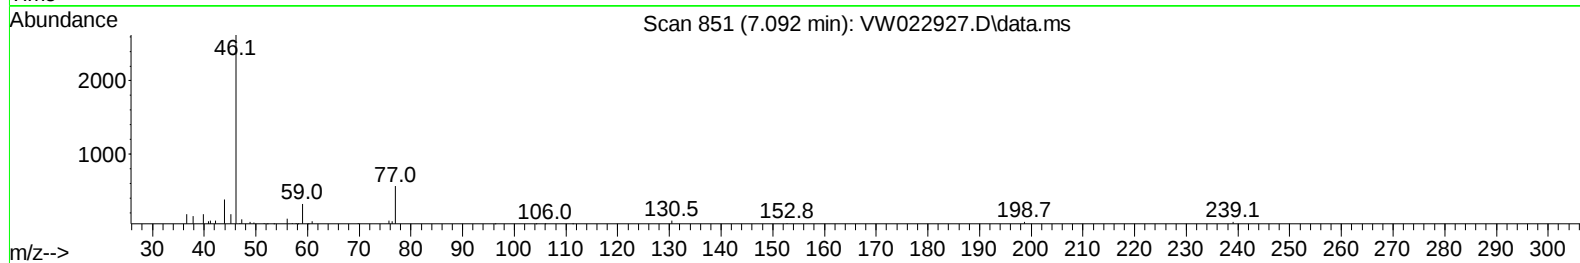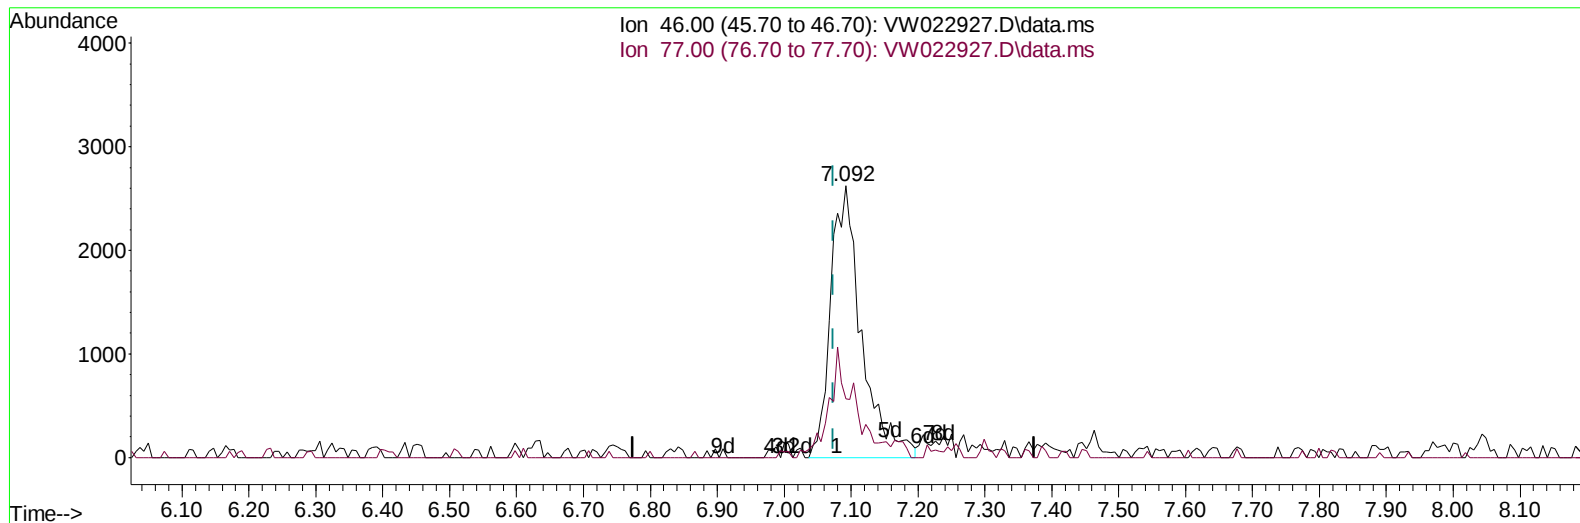

TIC: VW022927.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.018) 87.22 ug/L m

response 8369

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	19.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022927.D
 Acq On : 09 May 2022 14:04
 Operator : SY/VA
 Sample : N2713-08
 Misc : 6.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSK8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 09 22:57:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	24599	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	22148	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	10727	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	8706	17.250	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	69.000%	
7) Chloroethane-d5	2.885	69	9570	29.147	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	116.600%	
11) 1,1-Dichloroethene-d2	4.019	63	9433	14.465	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	57.880%	
21) 2-Butanone-d5	7.092	46	8369m	87.216	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	174.440%#	
24) Chloroform-d	7.659	84	15956	22.140	ug/L	0.01
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.560%	
26) 1,2-Dichloroethane-d4	8.305	65	10593	26.799	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	107.200%	
32) Benzene-d6	8.281	84	27258	21.352	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	85.400%	
36) 1,2-Dichloropropane-d6	9.274	67	8960	24.986	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	99.960%	
41) Toluene-d8	10.323	98	23118	18.746	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.000%	
43) trans-1,3-Dichloroprop...	10.585	79	3706	22.445	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.800%	
47) 2-Hexanone-d5	10.926	63	3457	50.500	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	101.000%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	12319	36.857	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	147.440%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	8659	23.092	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.360%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
Data File : VW022927.D
Acq On : 09 May 2022 14:04
Operator : SY/VA
Sample : N2713-08
Misc : 6.14g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSK8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 09 22:57:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 09 22:55:00 2022
Response via : Initial Calibration

