




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022938.D
 Acq On : 09 May 2022 18:28
 Operator : SY/VA
 Sample : N2714-05RE
 Misc : 4.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 09 23:00:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

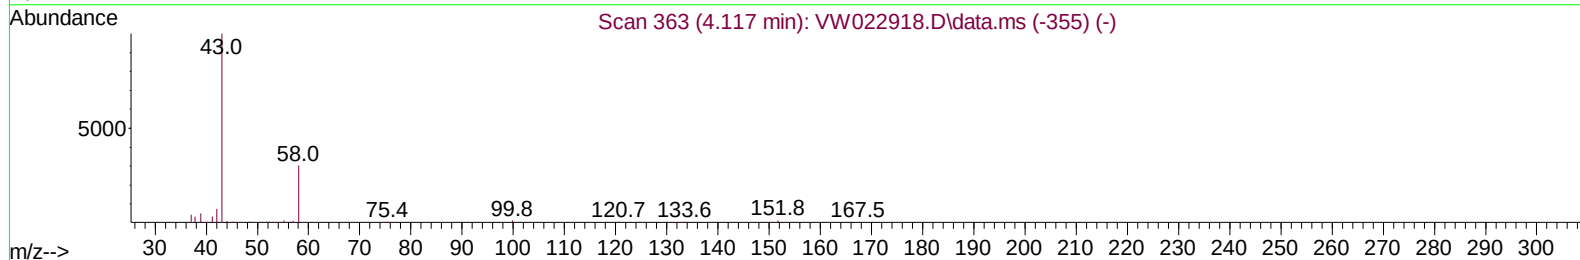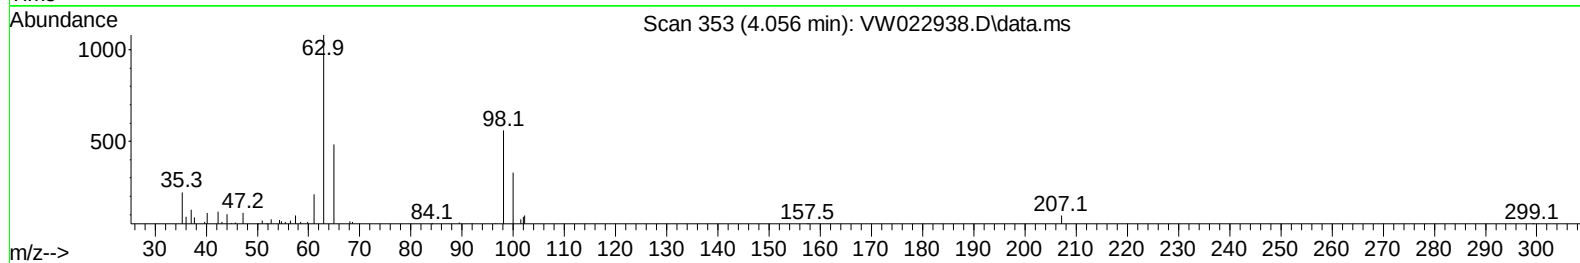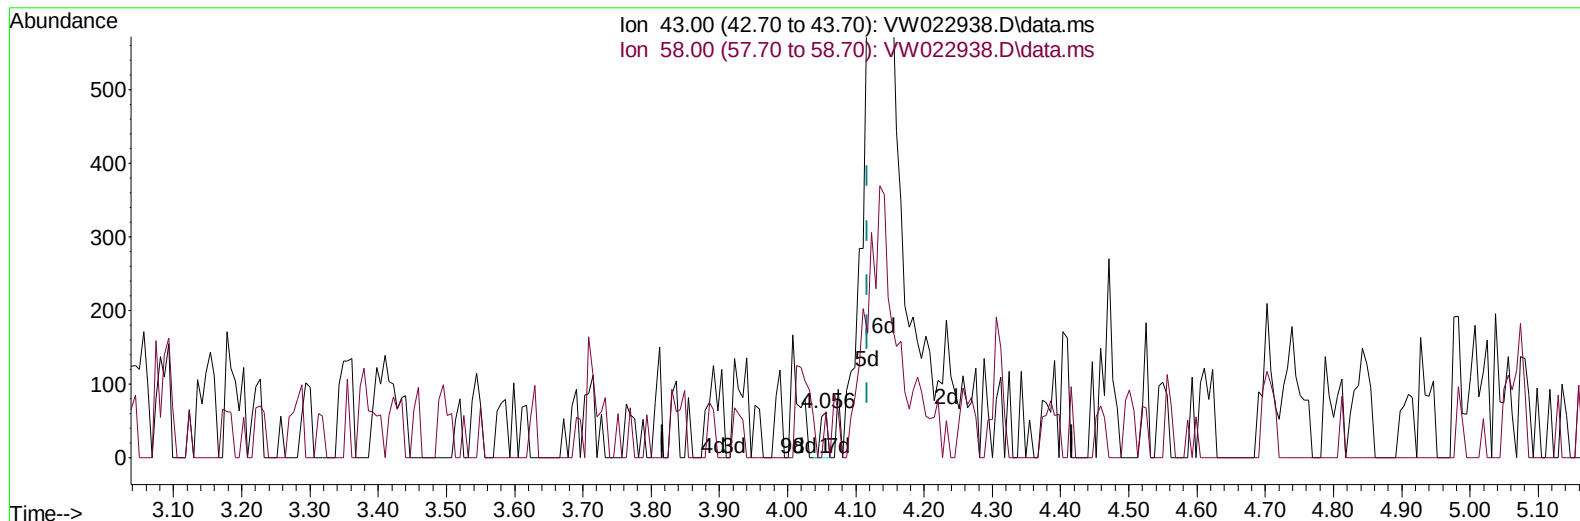

TIC: VW022938.D\data.ms

(13) Acetone (T)

4.056min (-0.061) 0.91 ug/L

response 42

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	54.76
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022938.D
 Acq On : 09 May 2022 18:28
 Operator : SY/VA
 Sample : N2714-05RE
 Misc : 4.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X6RE

Manual IntegrationsAPPROVED

Quant Time: May 09 23:00:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/10/2022

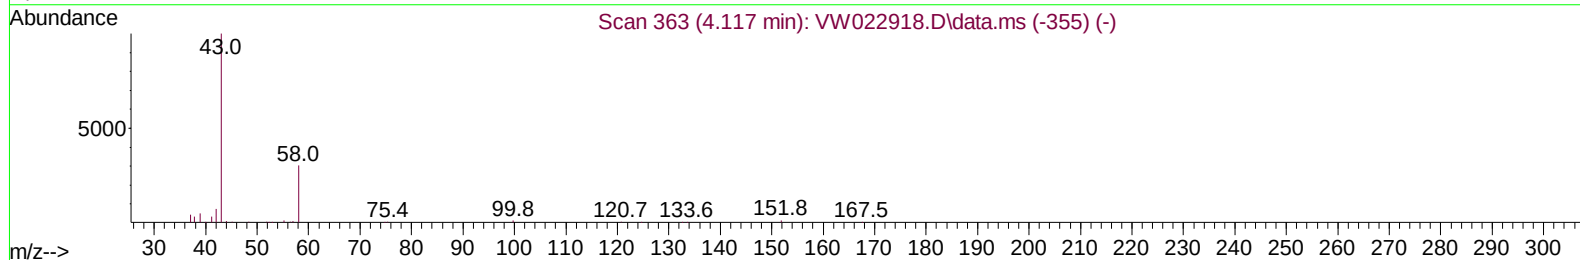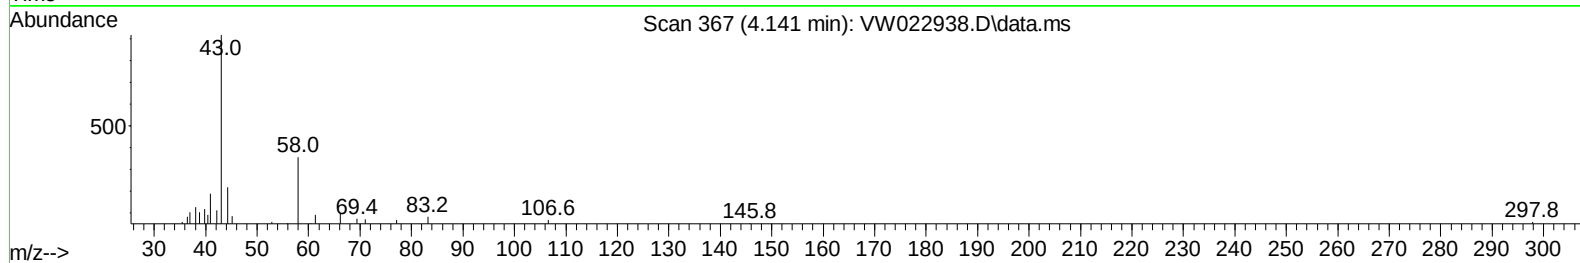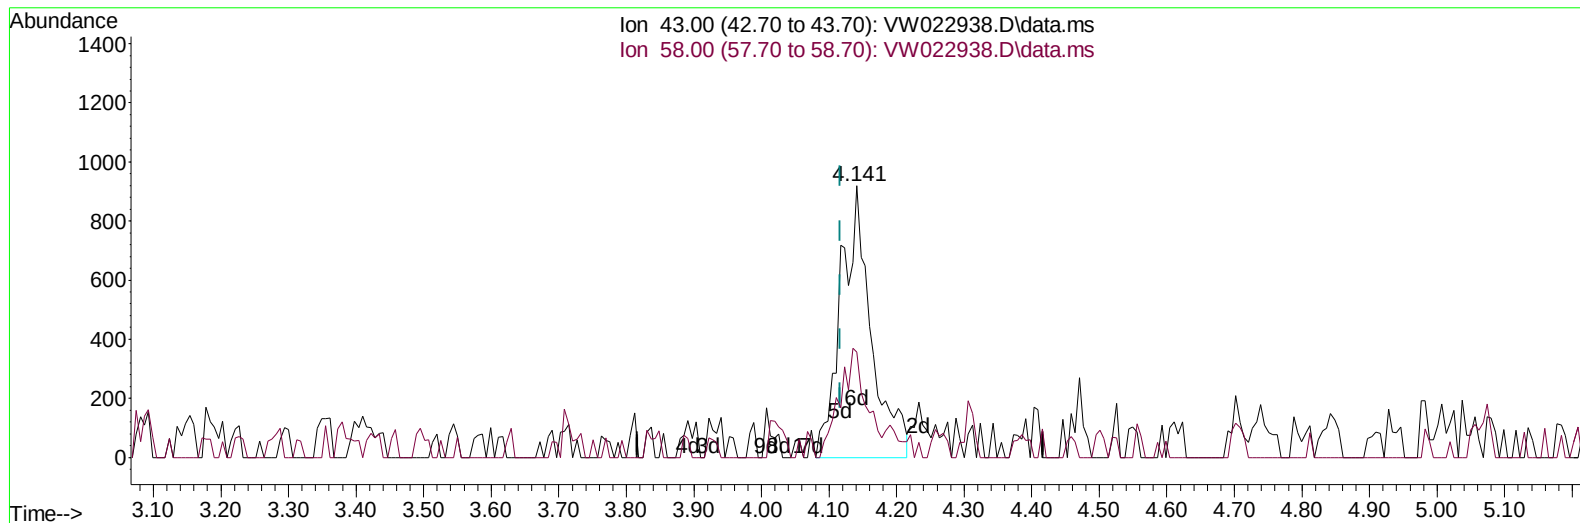

TIC: VW022938.D\data.ms

(13) Acetone (T)

4.141min (+ 0.025) 61.93 ug/L m

response 2872

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	0.80
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022938.D
 Acq On : 09 May 2022 18:28
 Operator : SY/VA
 Sample : N2714-05RE
 Misc : 4.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X6RE

Manual IntegrationsAPPROVED

Quant Time: May 09 23:00:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/10/2022

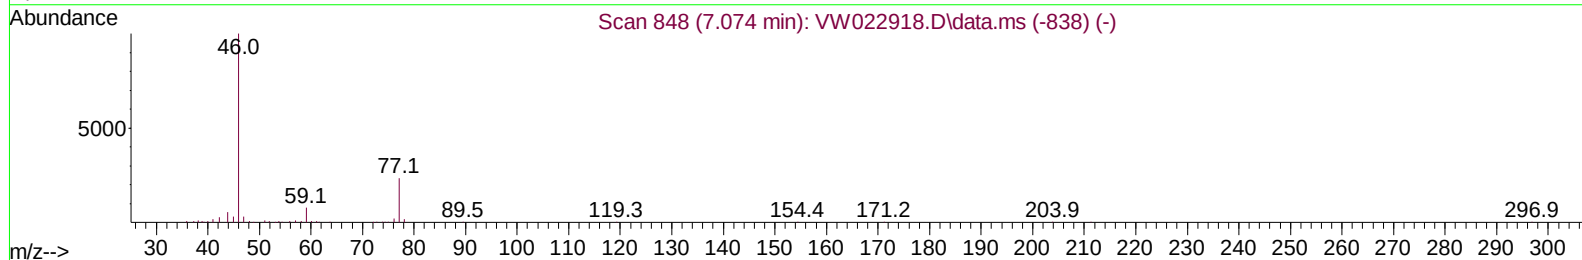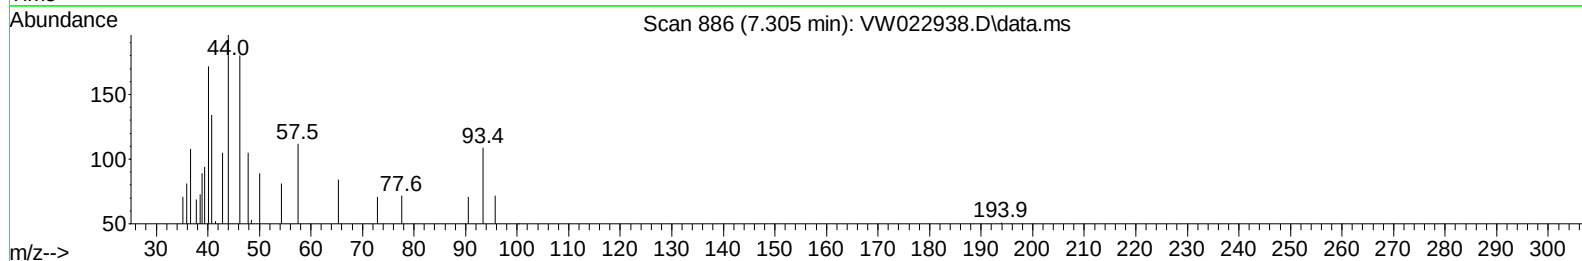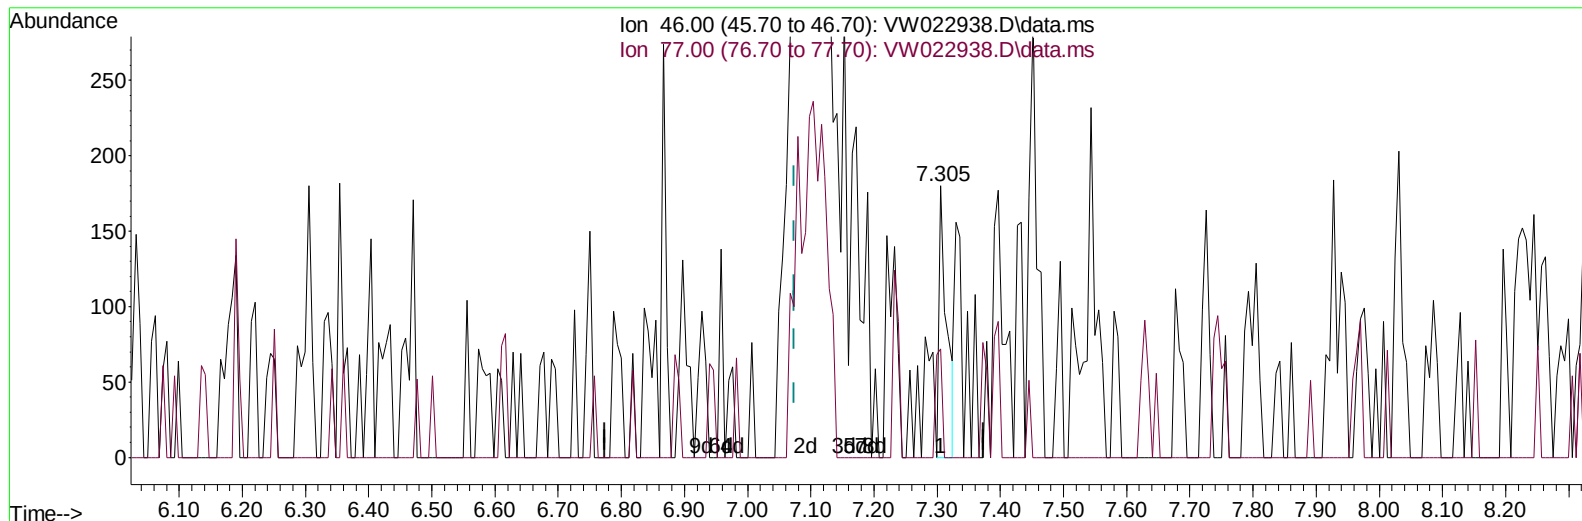

TIC: VW022938.D\data.ms

(21) 2-Butanone-d5 (S)

7.305min (+ 0.232) 2.49 ug/L

response 154

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	33.12
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022938.D
 Acq On : 09 May 2022 18:28
 Operator : SY/VA
 Sample : N2714-05RE
 Misc : 4.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X6RE

Manual IntegrationsAPPROVED

Quant Time: May 09 23:00:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/10/2022

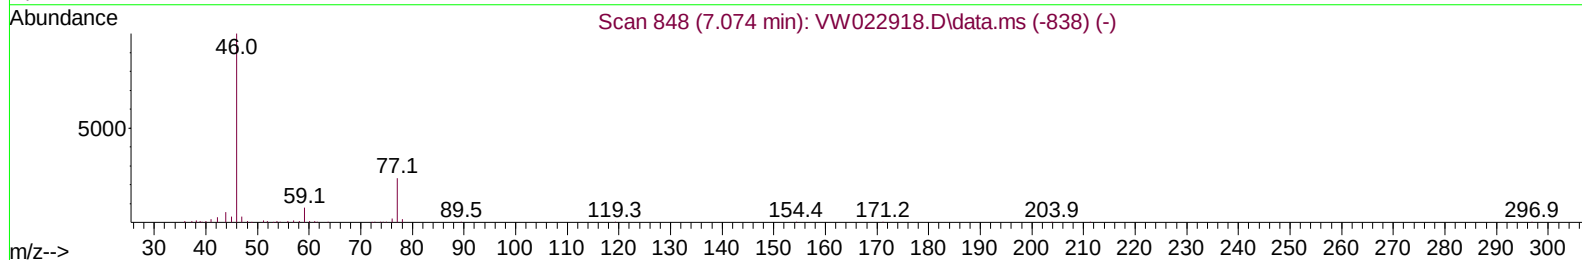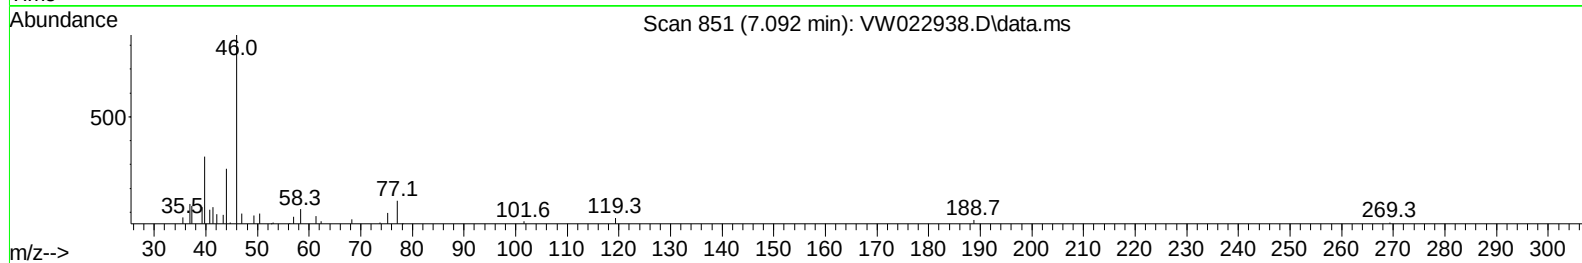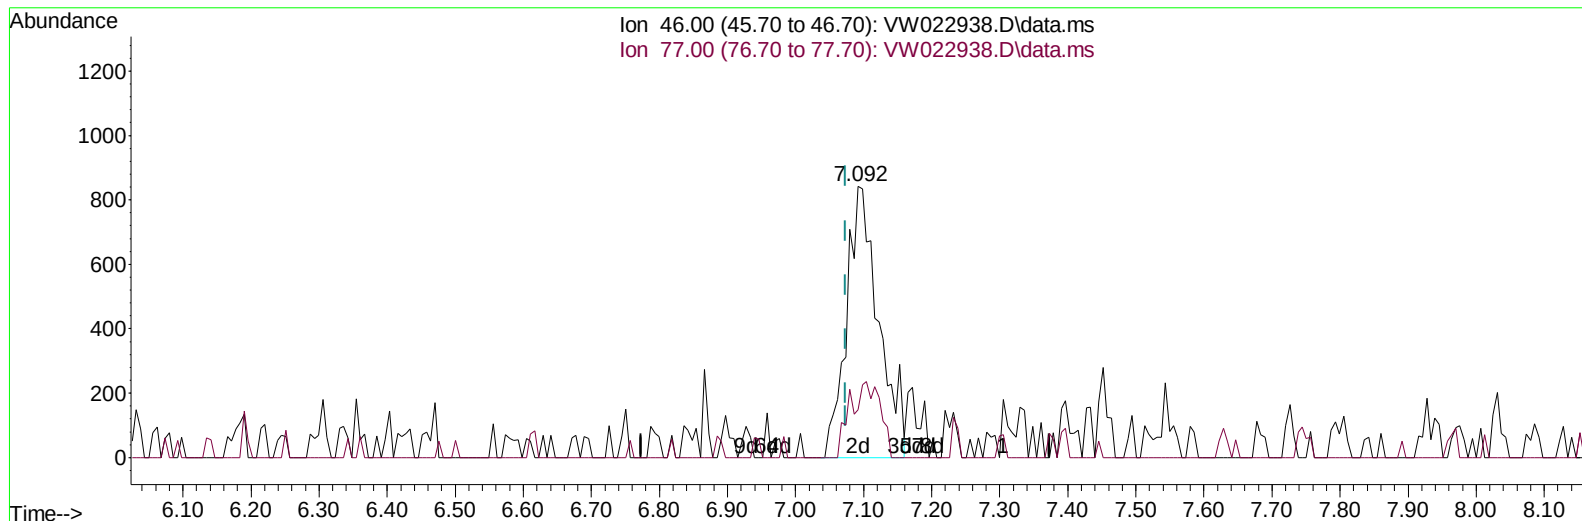

TIC: VW022938.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.018) 44.43 ug/L m

response 2752

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	1.85#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022938.D
 Acq On : 09 May 2022 18:28
 Operator : SY/VA
 Sample : N2714-05RE
 Misc : 4.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 09 23:00:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

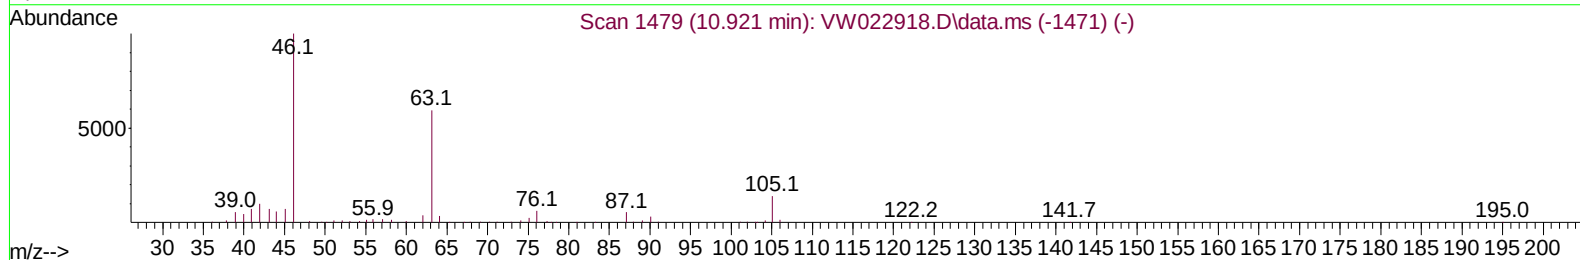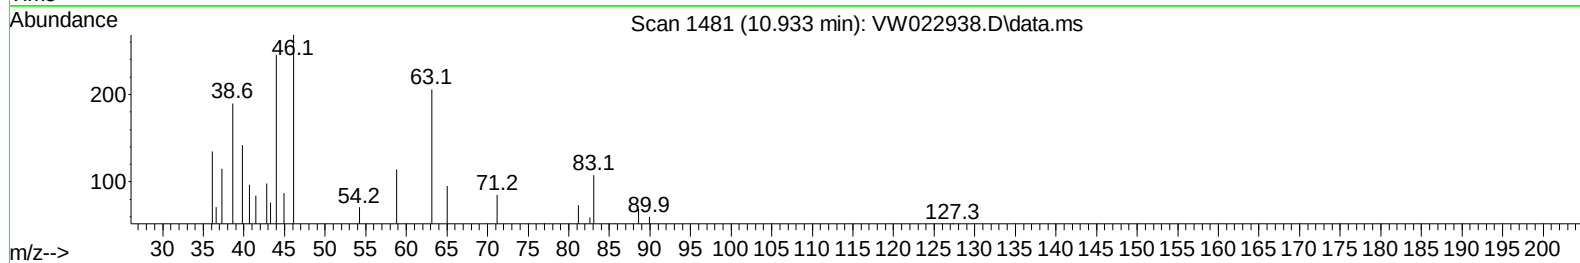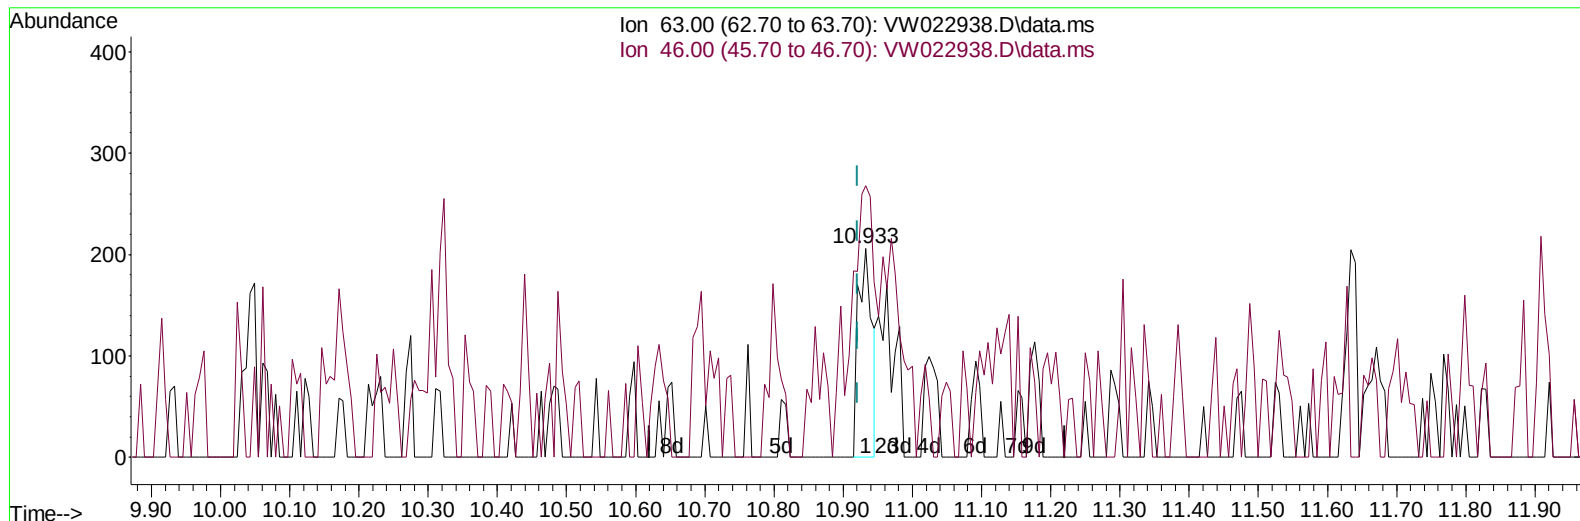

TIC: VW022938.D\data.ms

(47) 2-Hexanone-d5 (S)

10.933min (+ 0.012) 6.85 ug/L

response 290

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	166.00	197.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
Data File : VW022938.D
Acq On : 09 May 2022 18:28
Operator : SY/VA
Sample : N2714-05RE
Misc : 4.48g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW2X6RE

Manual IntegrationsAPPROVED

Quant Time: May 09 23:00:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 09 22:55:00 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/10/2022

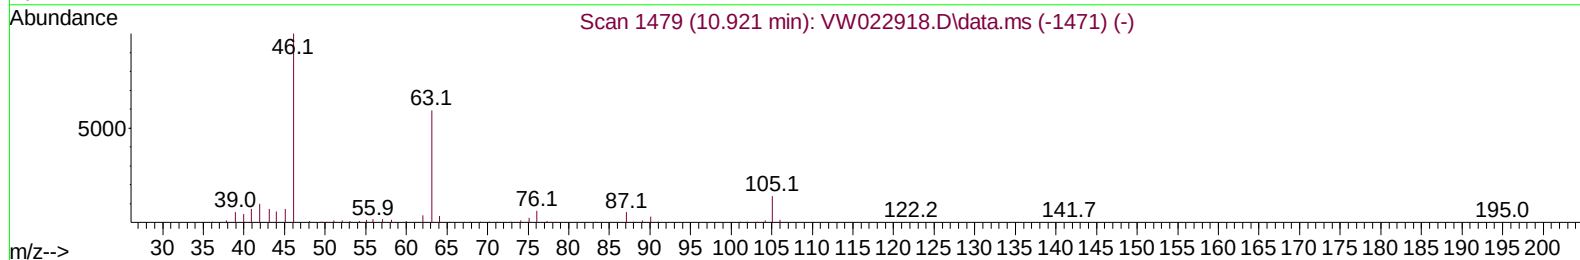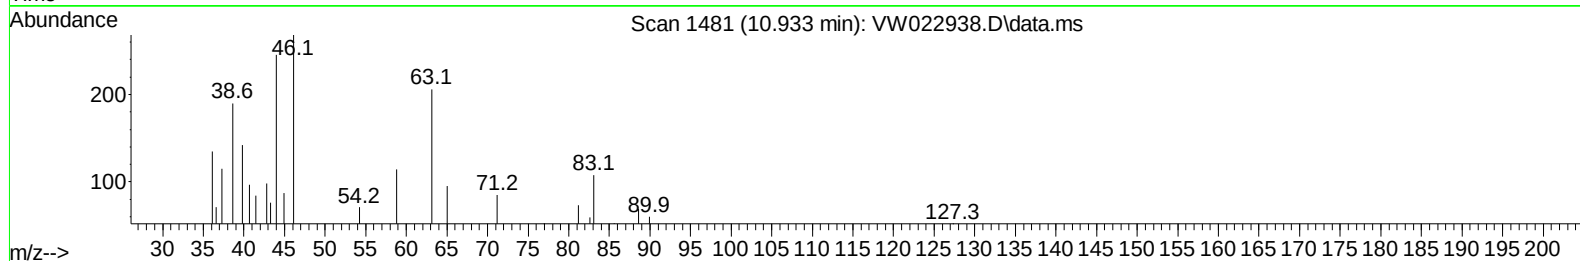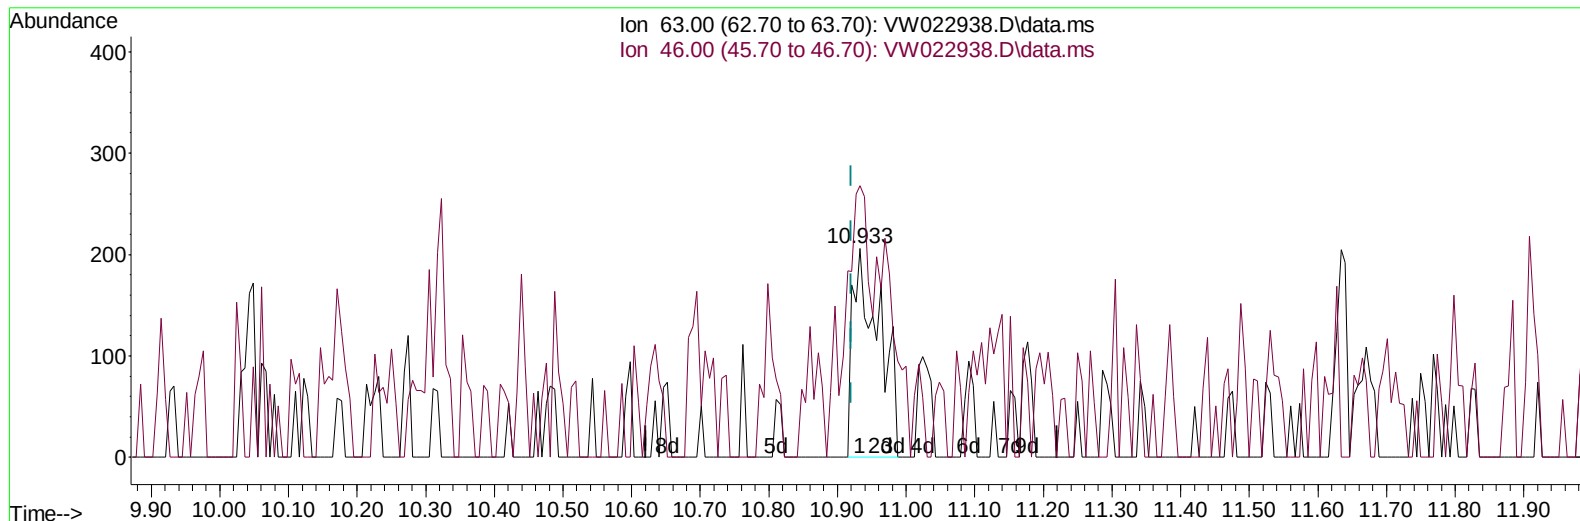

TIC: VW022938.D\data.ms

(47) 2-Hexanone-d5 (S)

10.933min (+ 0.012) 13.09 ug/L m

response 554

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	166.00	103.25#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022938.D
 Acq On : 09 May 2022 18:28
 Operator : SY/VA
 Sample : N2714-05RE
 Misc : 4.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 09 23:00:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	15878	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	13695	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	3491	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	6480	19.892	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	79.560%		
7) Chloroethane-d5	2.898	69	4354	20.544	ug/L	0.01
Spiked Amount 25.000	Range 30	- 150	Recovery =	82.160%		
11) 1,1-Dichloroethene-d2	4.032	63	6784	16.117	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	64.480%		
21) 2-Butanone-d5	7.092	46	2752m	44.432	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery =	88.860%		
24) Chloroform-d	7.653	84	10831	23.283	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	93.120%		
26) 1,2-Dichloroethane-d4	8.311	65	6508	25.508	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	102.040%		
32) Benzene-d6	8.275	84	18911	23.957	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	95.840%		
36) 1,2-Dichloropropane-d6	9.281	67	6303	28.426	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	113.720%		
41) Toluene-d8	10.329	98	15259	20.011	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	80.040%		
43) trans-1,3-Dichloroprop...	10.585	79	1952	19.119	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	76.480%		
47) 2-Hexanone-d5	10.933	63	554m	13.088	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery =	26.180%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	4176	20.206	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	80.840%		
66) 1,2-Dichlorobenzene-d4	13.847	152	2713	22.232	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	88.920%		
Target Compounds						
13) Acetone	4.141	43	2872m	61.934	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
Data File : VW022938.D
Acq On : 09 May 2022 18:28
Operator : SY/VA
Sample : N2714-05RE
Misc : 4.48g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW2X6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 09 23:00:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 09 22:55:00 2022
Response via : Initial Calibration

