

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
 Data File : VW022938.D
 Acq On : 09 May 2022 18:28
 Operator : SY/VA
 Sample : N2714-05RE
 Misc : 4.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW2X6RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
 Supervised By :Mahesh Dadoda 05/10/2022

Quant Time: May 09 23:00:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon May 09 22:55:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	15878	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	13695	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	3491	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	6480	19.892	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.560%
7) Chloroethane-d5	2.898	69	4354	20.544	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.160%
11) 1,1-Dichloroethene-d2	4.032	63	6784	16.117	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.480%
21) 2-Butanone-d5	7.092	46	2752m	44.432	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.860%
24) Chloroform-d	7.653	84	10831	23.283	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.120%
26) 1,2-Dichloroethane-d4	8.311	65	6508	25.508	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.040%
32) Benzene-d6	8.275	84	18911	23.957	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.840%
36) 1,2-Dichloropropane-d6	9.281	67	6303	28.426	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.720%
41) Toluene-d8	10.329	98	15259	20.011	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.040%
43) trans-1,3-Dichloroprop...	10.585	79	1952	19.119	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.480%
47) 2-Hexanone-d5	10.933	63	554m	13.088	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	26.180%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	4176	20.206	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.840%
66) 1,2-Dichlorobenzene-d4	13.847	152	2713	22.232	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.920%
Target Compounds					Qvalue	
13) Acetone	4.141	43	2872m	61.934	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050922\
Data File : VW022938.D
Acq On : 09 May 2022 18:28
Operator : SY/VA
Sample : N2714-05RE
Misc : 4.48g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW2X6RE

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/10/2022
Supervised By : Mahesh Dadoda 05/10/2022


Quant Time: May 09 23:00:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Mon May 09 22:55:00 2022
Response via : Initial Calibration

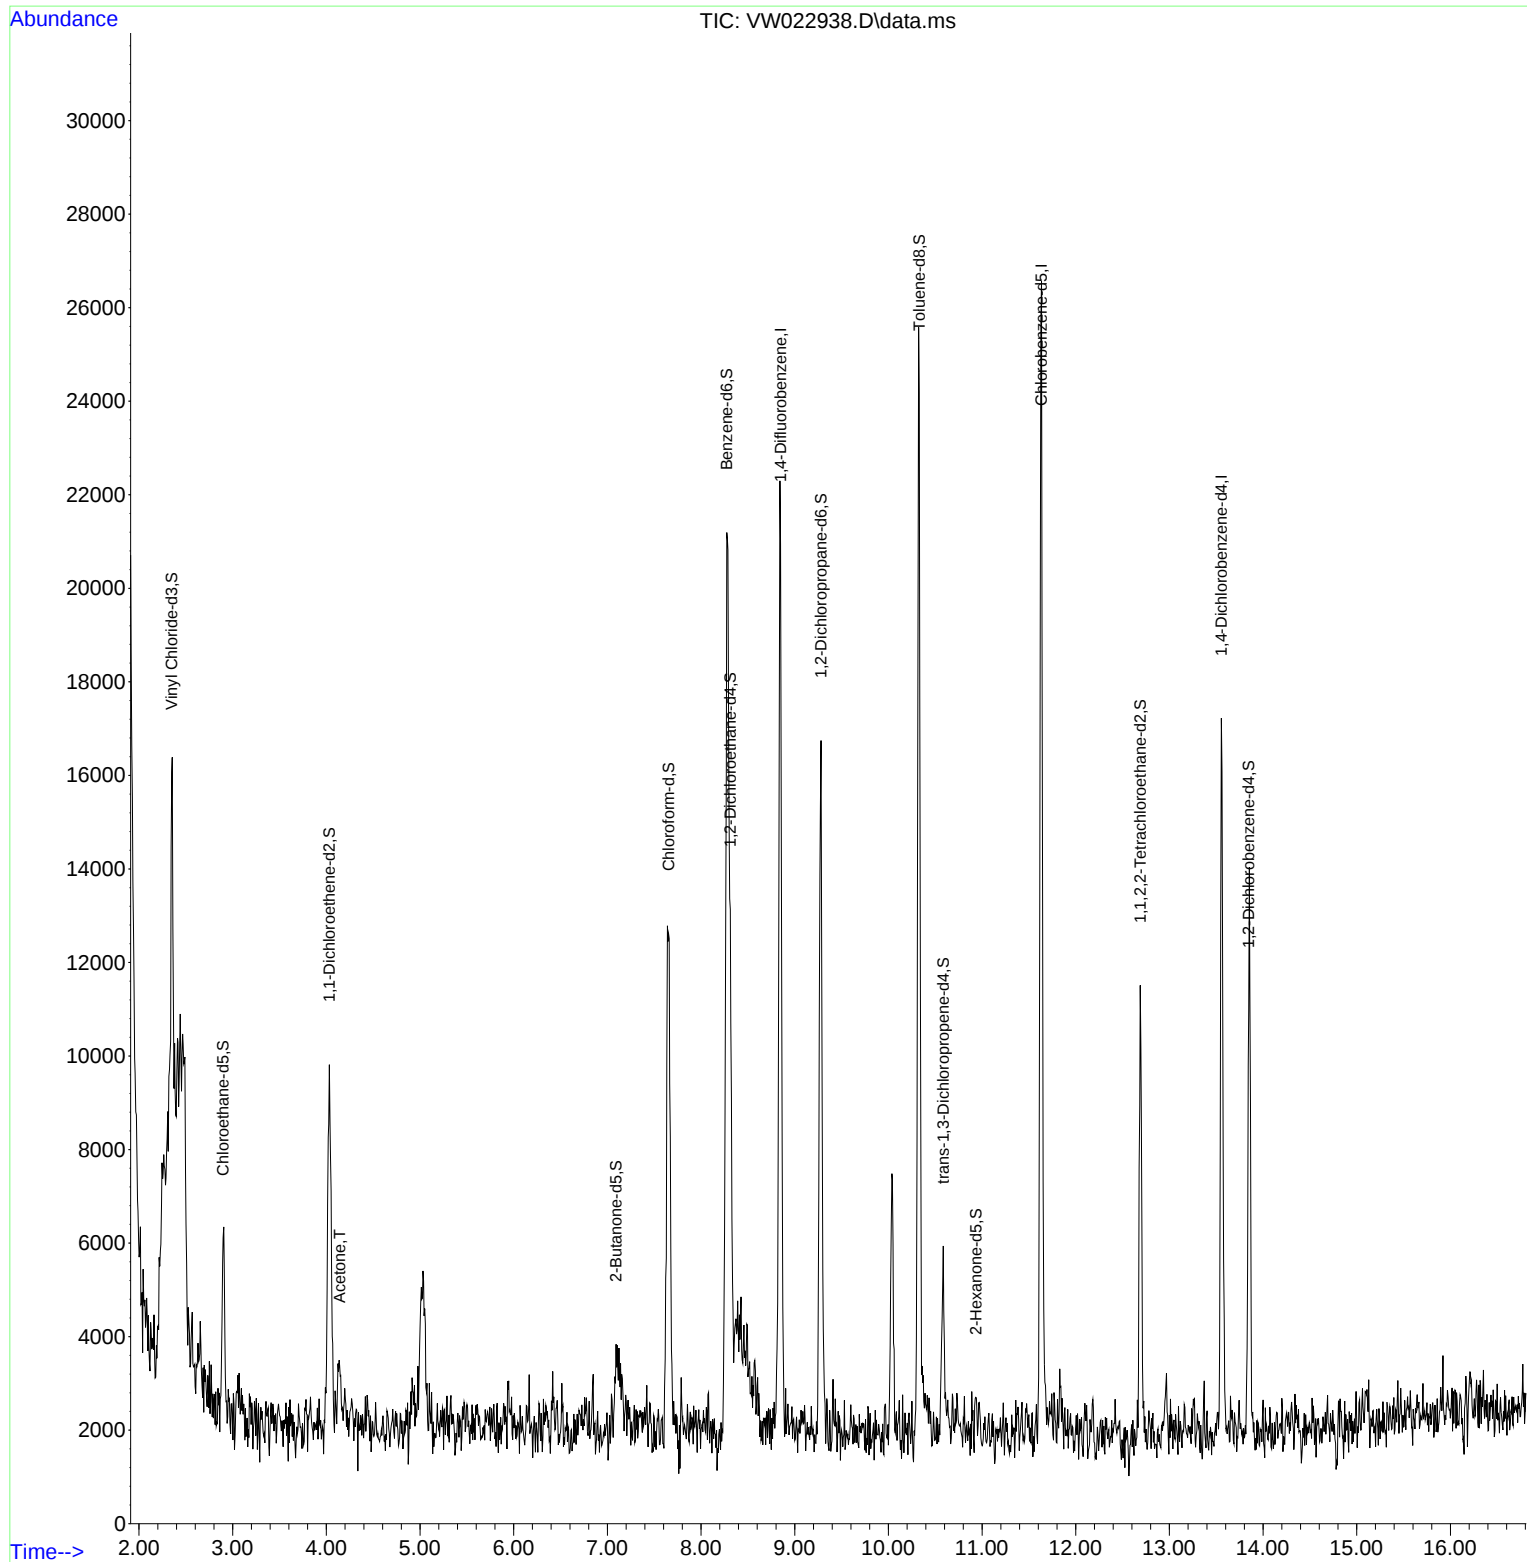

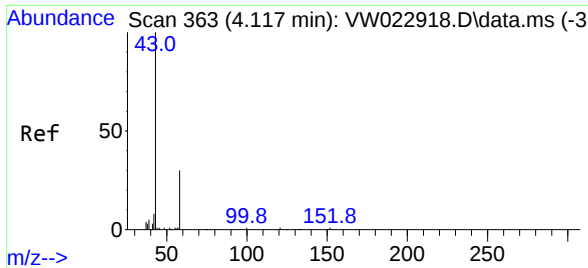

#13
Acetone
Concen: 61.934 ug/L m
RT: 4.141 min Scan# 30
Delta R.T. 0.025 min
Lab File: VW022938.D
Acq: 09 May 2022 18:28

Instrument :
MSVOA_W
ClientSampleId :
EW2X6RE

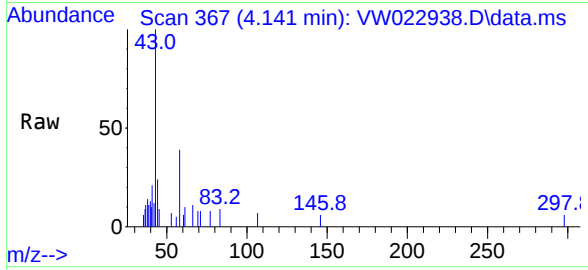

Tgt Ion: 43 Resp: 2872
Ion Ratio Lower Upper
43 100
58 0.8 0.0 64.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/10/2022
Supervised By :Mahesh Dadoda 05/10/2022

