




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051023\
 Data File : VW025927.D
 Acq On : 10 May 2023 14:06
 Operator : SY/MD
 Sample : 02664-10
 Misc : 5.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JREA5

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/11/2023
 Supervised By :Mahesh Dadoda 05/11/2023

Quant Time: May 11 02:12:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

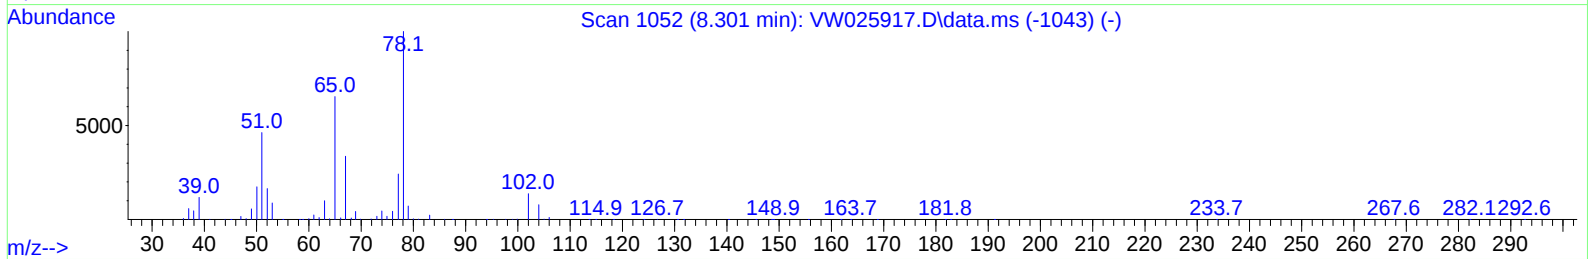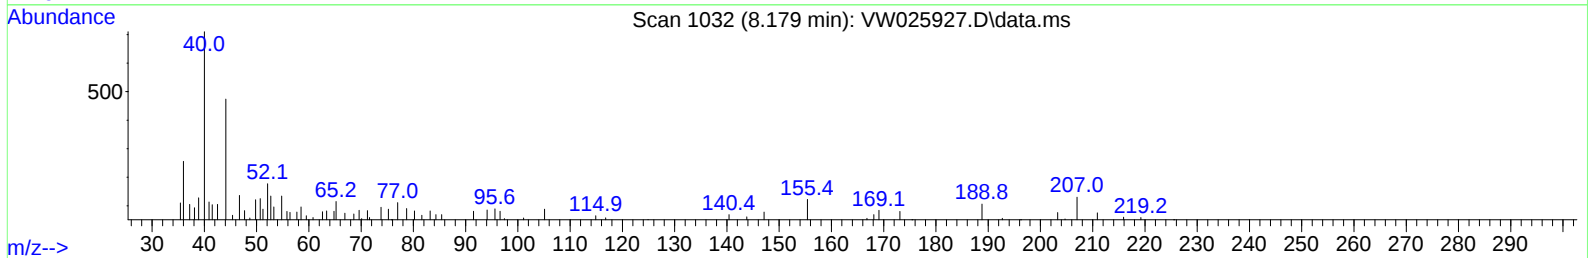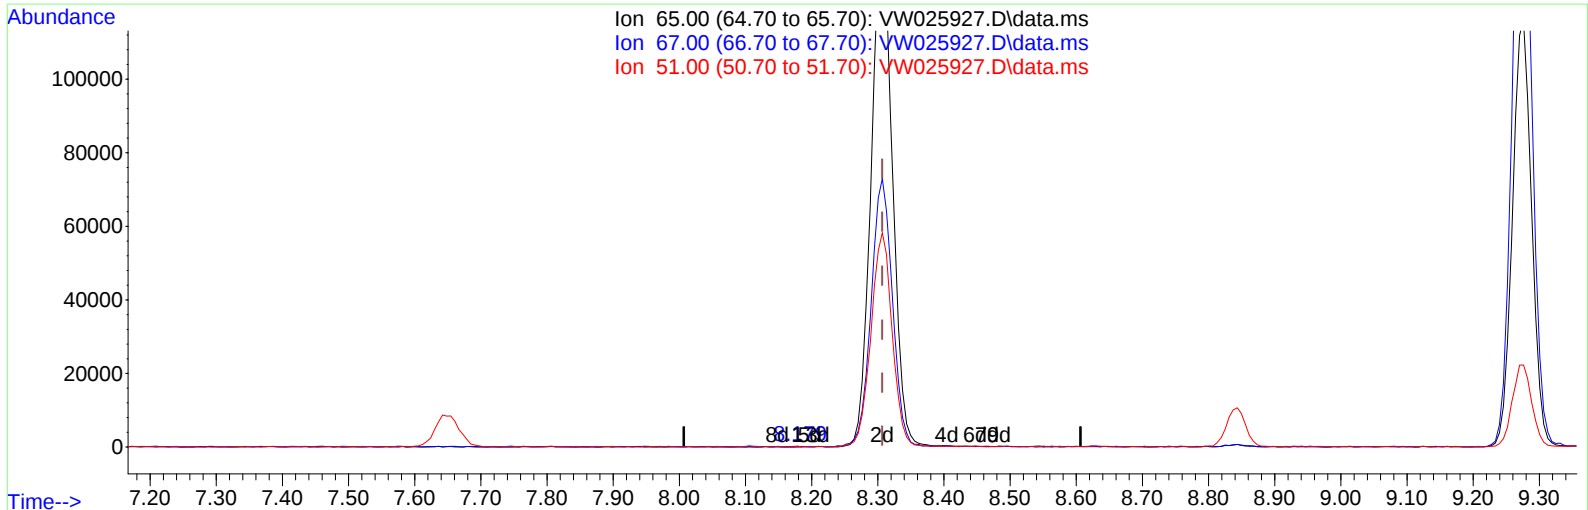

TIC: VW025927.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.179min (-0.128) 0.01 ug/L

response 168

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	53.57
51.00	112.30	85.71
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051023\
 Data File : VW025927.D
 Acq On : 10 May 2023 14:06
 Operator : SY/MD
 Sample : 02664-10
 Misc : 5.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JREA5

Manual IntegrationsAPPROVED

Quant Time: May 11 02:12:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/11/2023
 Supervised By :Mahesh Dadoda 05/11/2023

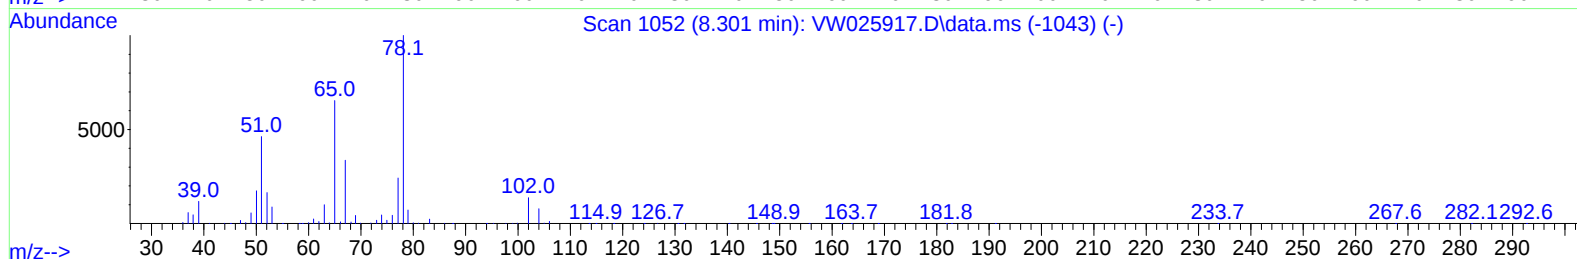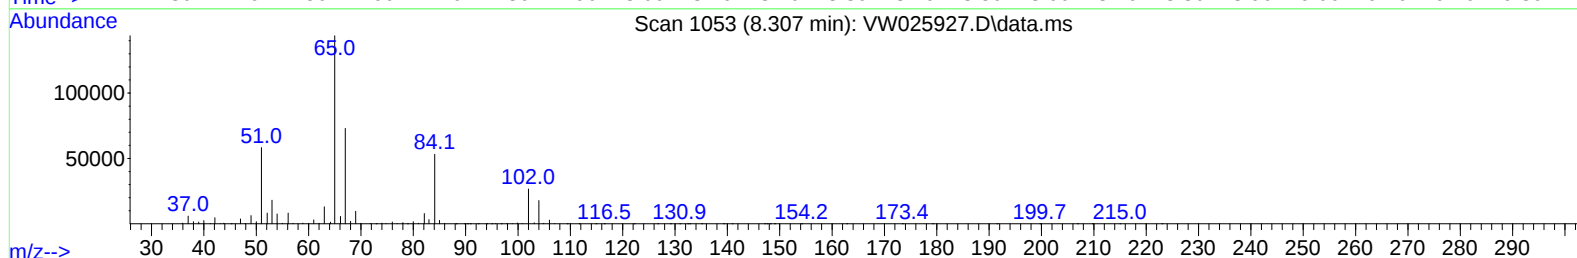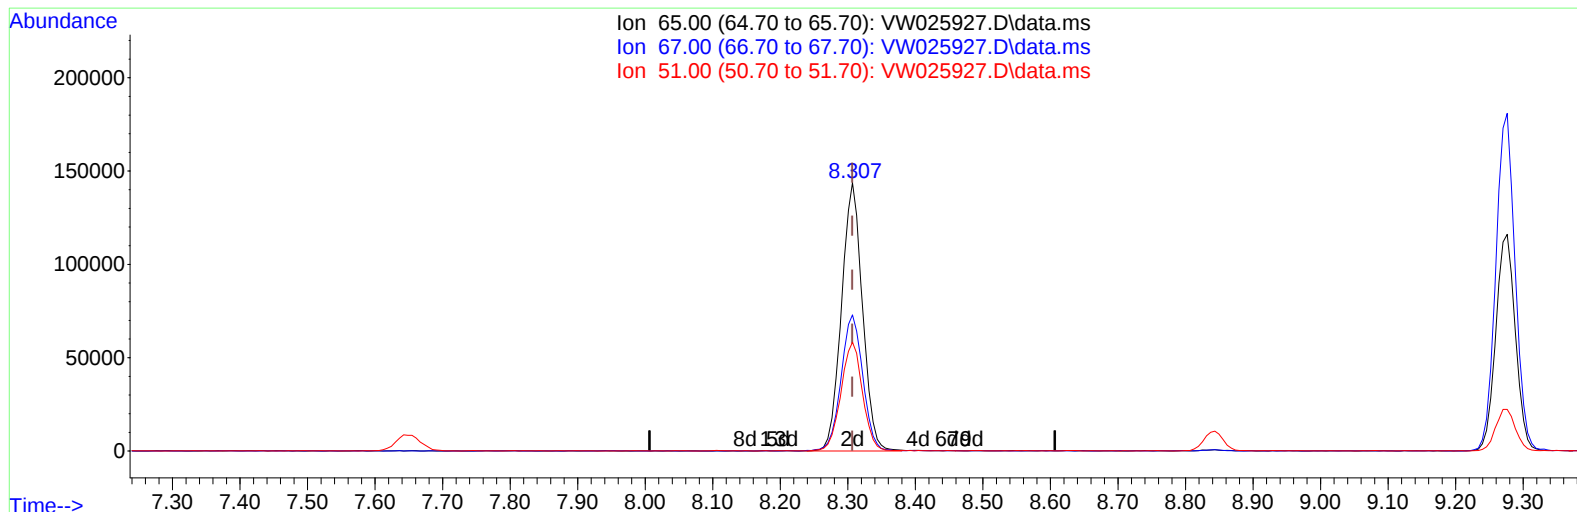

TIC: VW025927.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 21.06 ug/L m

response 309983

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.03#
51.00	112.30	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051023\
 Data File : VW025927.D
 Acq On : 10 May 2023 14:06
 Operator : SY/MD
 Sample : 02664-10
 Misc : 5.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JREA5

Manual IntegrationsAPPROVED

Quant Time: May 11 02:12:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/11/2023
 Supervised By :Mahesh Dadoda 05/11/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	902657	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	663067	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	171386	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	261023	20.406	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.640%		
7) Chloroethane-d5	2.893	69	211170	22.268	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.080%		
11) 1,1-Dichloroethene-d2	4.021	65	126191	19.702	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	78.800%		
21) 2-Butanone-d5	7.081	46	170523	40.326	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	80.660%		
24) Chloroform-d	7.648	84	540545	20.768	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	83.080%		
26) 1,2-Dichloroethane-d4	8.307	65	309983m	21.061	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	84.240%		
32) Benzene-d6	8.276	84	1103013	25.458	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	101.840%		
36) 1,2-Dichloropropane-d6	9.276	67	359746	25.951	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	103.800%		
41) Toluene-d8	10.325	98	886756	22.952	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	91.800%		
43) trans-1,3-Dichloroprop...	10.575	79	119847	21.328	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.320%		
47) 2-Hexanone-d5	10.922	63	113370	47.961	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.920%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	212998	20.159	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	80.640%		
66) 1,2-Dichlorobenzene-d4	13.849	152	123939	19.837	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	79.360%		
Target Compounds					Qvalue	
13) Acetone	4.137	43	16229	4.328	ug/L	94
16) Methylene chloride	4.923	84	42628	2.290	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051023\
Data File : VW025927.D
Acq On : 10 May 2023 14:06
Operator : SY/MD
Sample : 02664-10
Misc : 5.60g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JREA5

Manual IntegrationsAPPROVED

Quant Time: May 11 02:12:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 05 23:47:36 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/11/2023
Supervised By :Mahesh Dadoda 05/11/2023

