

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
 Data File : VW022968.D
 Acq On : 11 May 2022 10:06
 Operator : SY/VA
 Sample : N2708-23
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: May 12 01:08:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 12 01:07:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	305829	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	300287	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	150783	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	115457	18.401	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.600%
7) Chloroethane-d5	2.885	69	85617	20.974	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.880%
11) 1,1-Dichloroethene-d2	4.019	63	121612	15.000	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.000%
21) 2-Butanone-d5	7.079	46	58820	49.305	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.600%
24) Chloroform-d	7.646	84	215965	24.103	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.400%
26) 1,2-Dichloroethane-d4	8.433	65	116	0.024	ug/L	0.13
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.274	84	406612	23.492	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.960%
36) 1,2-Dichloropropane-d6	9.274	67	122923	25.283	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.120%
41) Toluene-d8	10.323	98	378654	22.647	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.600%
43) trans-1,3-Dichloroprop...	10.579	79	47964	21.425	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.720%
47) 2-Hexanone-d5	10.920	63	43419	46.781	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.560%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	110451	24.373	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.480%
66) 1,2-Dichlorobenzene-d4	13.853	152	131756	24.997	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.000%
Target Compounds						Qvalue
35) Methylcyclohexane	9.274	83	31732	3.970	ug/L	# 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
Data File : VW022968.D
Acq On : 11 May 2022 10:06
Operator : SY/VA
Sample : N2708-23
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: May 12 01:08:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 12 01:07:03 2022
Response via : Initial Calibration

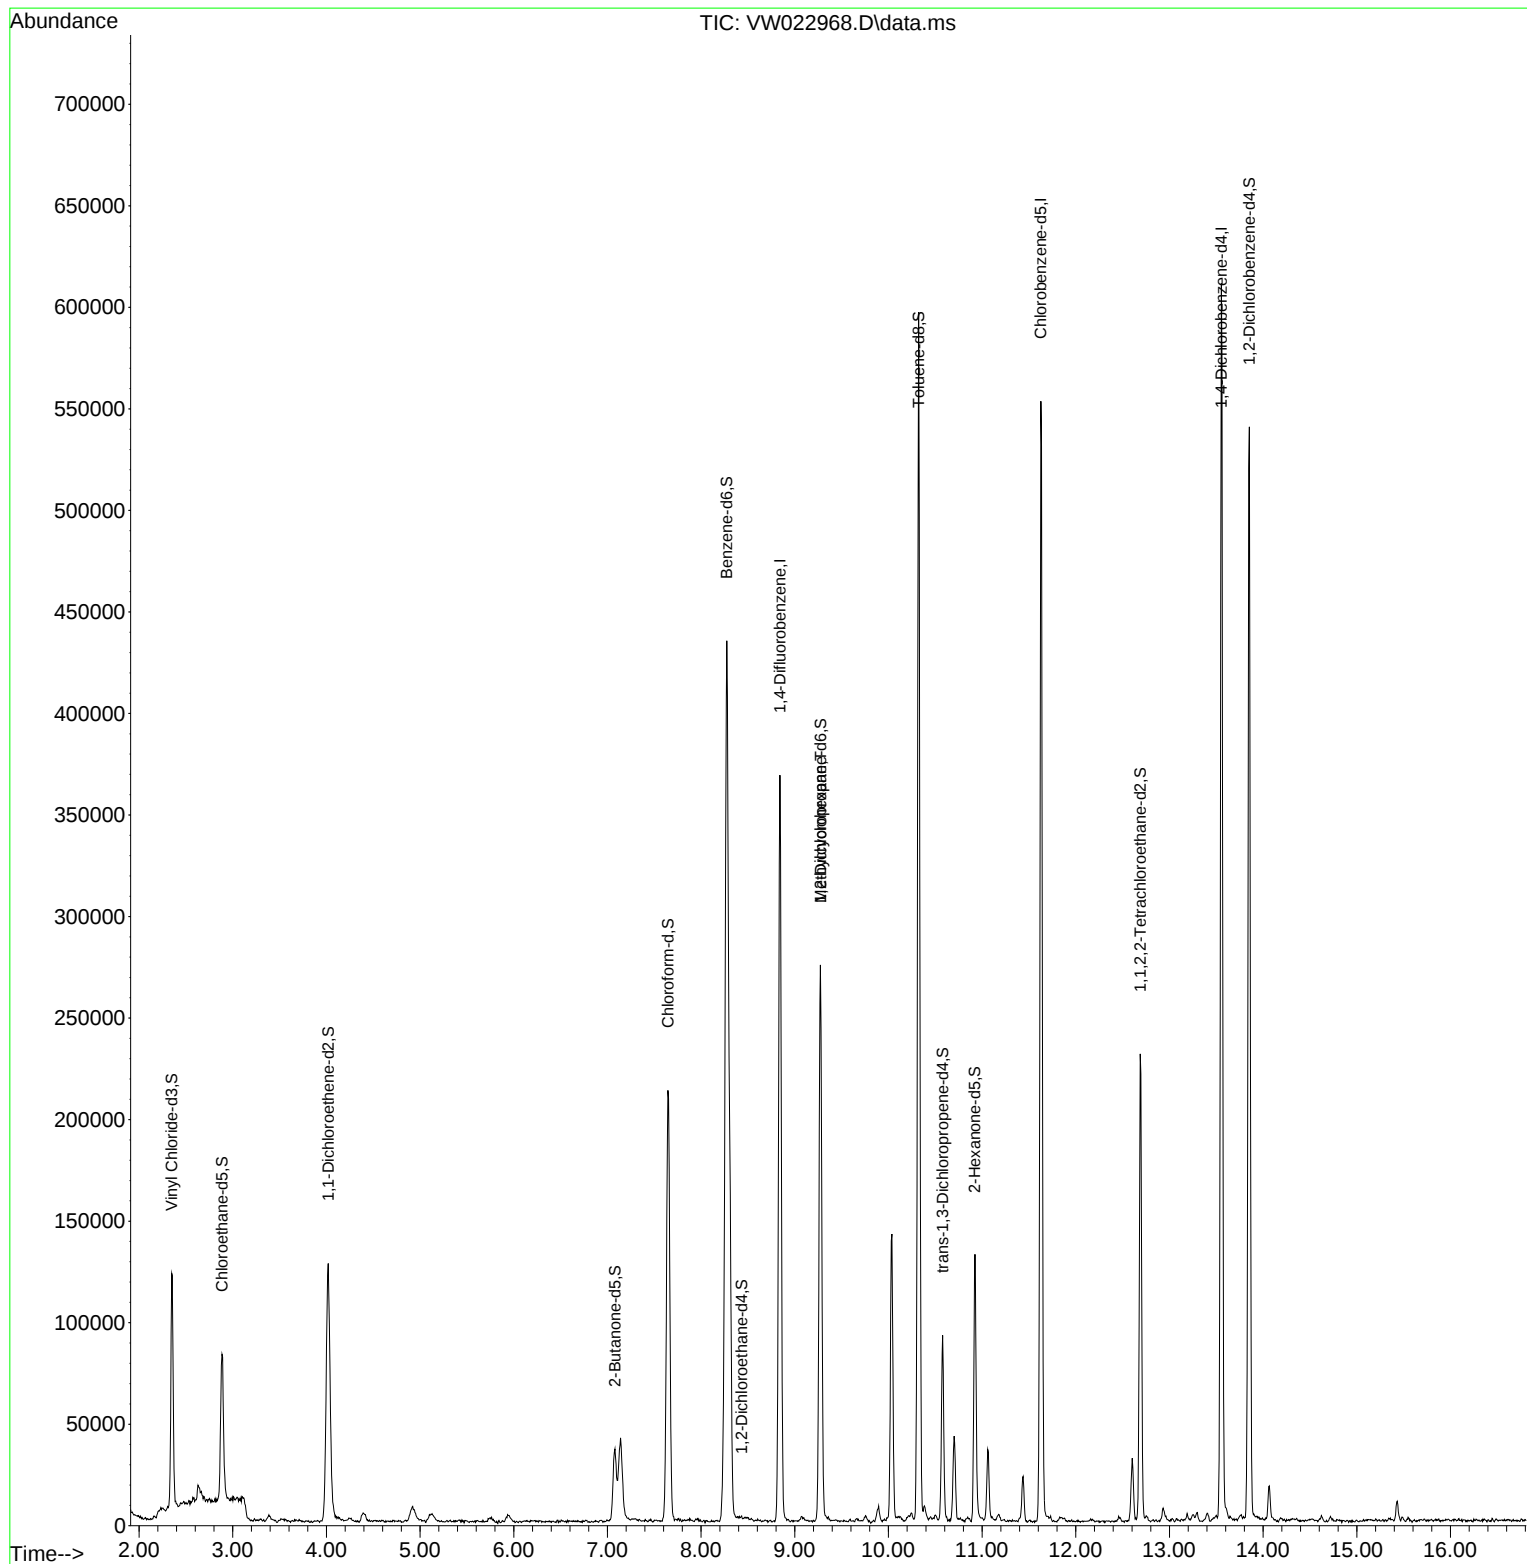

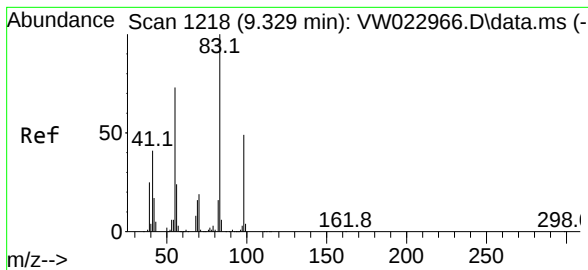

#35
 Methylcyclohexane
 Concen: 3.970 ug/L
 RT: 9.274 min Scan# 11
 Delta R.T. -0.055 min
 Lab File: VW022968.D
 Acq: 11 May 2022 10:06

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 83	Resp:	31732
Ion Ratio	Lower	Upper
83	100	
55	0.6	55.1 82.7#
98	2.9	40.4 60.6#

