

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
 Data File : VW022969.D
 Acq On : 11 May 2022 10:30
 Operator : SY/VA
 Sample : N2713-09
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: May 12 01:08:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 12 01:07:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	300167	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	296671	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	146343	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	106938	17.365	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.440%
7) Chloroethane-d5	2.886	69	85708	21.392	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.560%
11) 1,1-Dichloroethene-d2	4.019	63	117140	14.721	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.880%
21) 2-Butanone-d5	7.074	46	64543	55.122	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.240%
24) Chloroform-d	7.653	84	209532	23.826	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.320%
26) 1,2-Dichloroethane-d4	8.305	65	119383	24.751	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.000%
32) Benzene-d6	8.275	84	396439	23.184	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.720%
36) 1,2-Dichloropropane-d6	9.275	67	120615	25.110	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.440%
41) Toluene-d8	10.323	98	370616	22.436	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.760%
43) trans-1,3-Dichloroprop...	10.579	79	48772	22.052	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.200%
47) 2-Hexanone-d5	10.921	63	49992	54.519	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.040%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	114036	25.471	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	129460	25.307	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.240%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.031	75	4385	0.669	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
Data File : VW022969.D
Acq On : 11 May 2022 10:30
Operator : SY/VA
Sample : N2713-09
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: May 12 01:08:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 12 01:07:03 2022
Response via : Initial Calibration

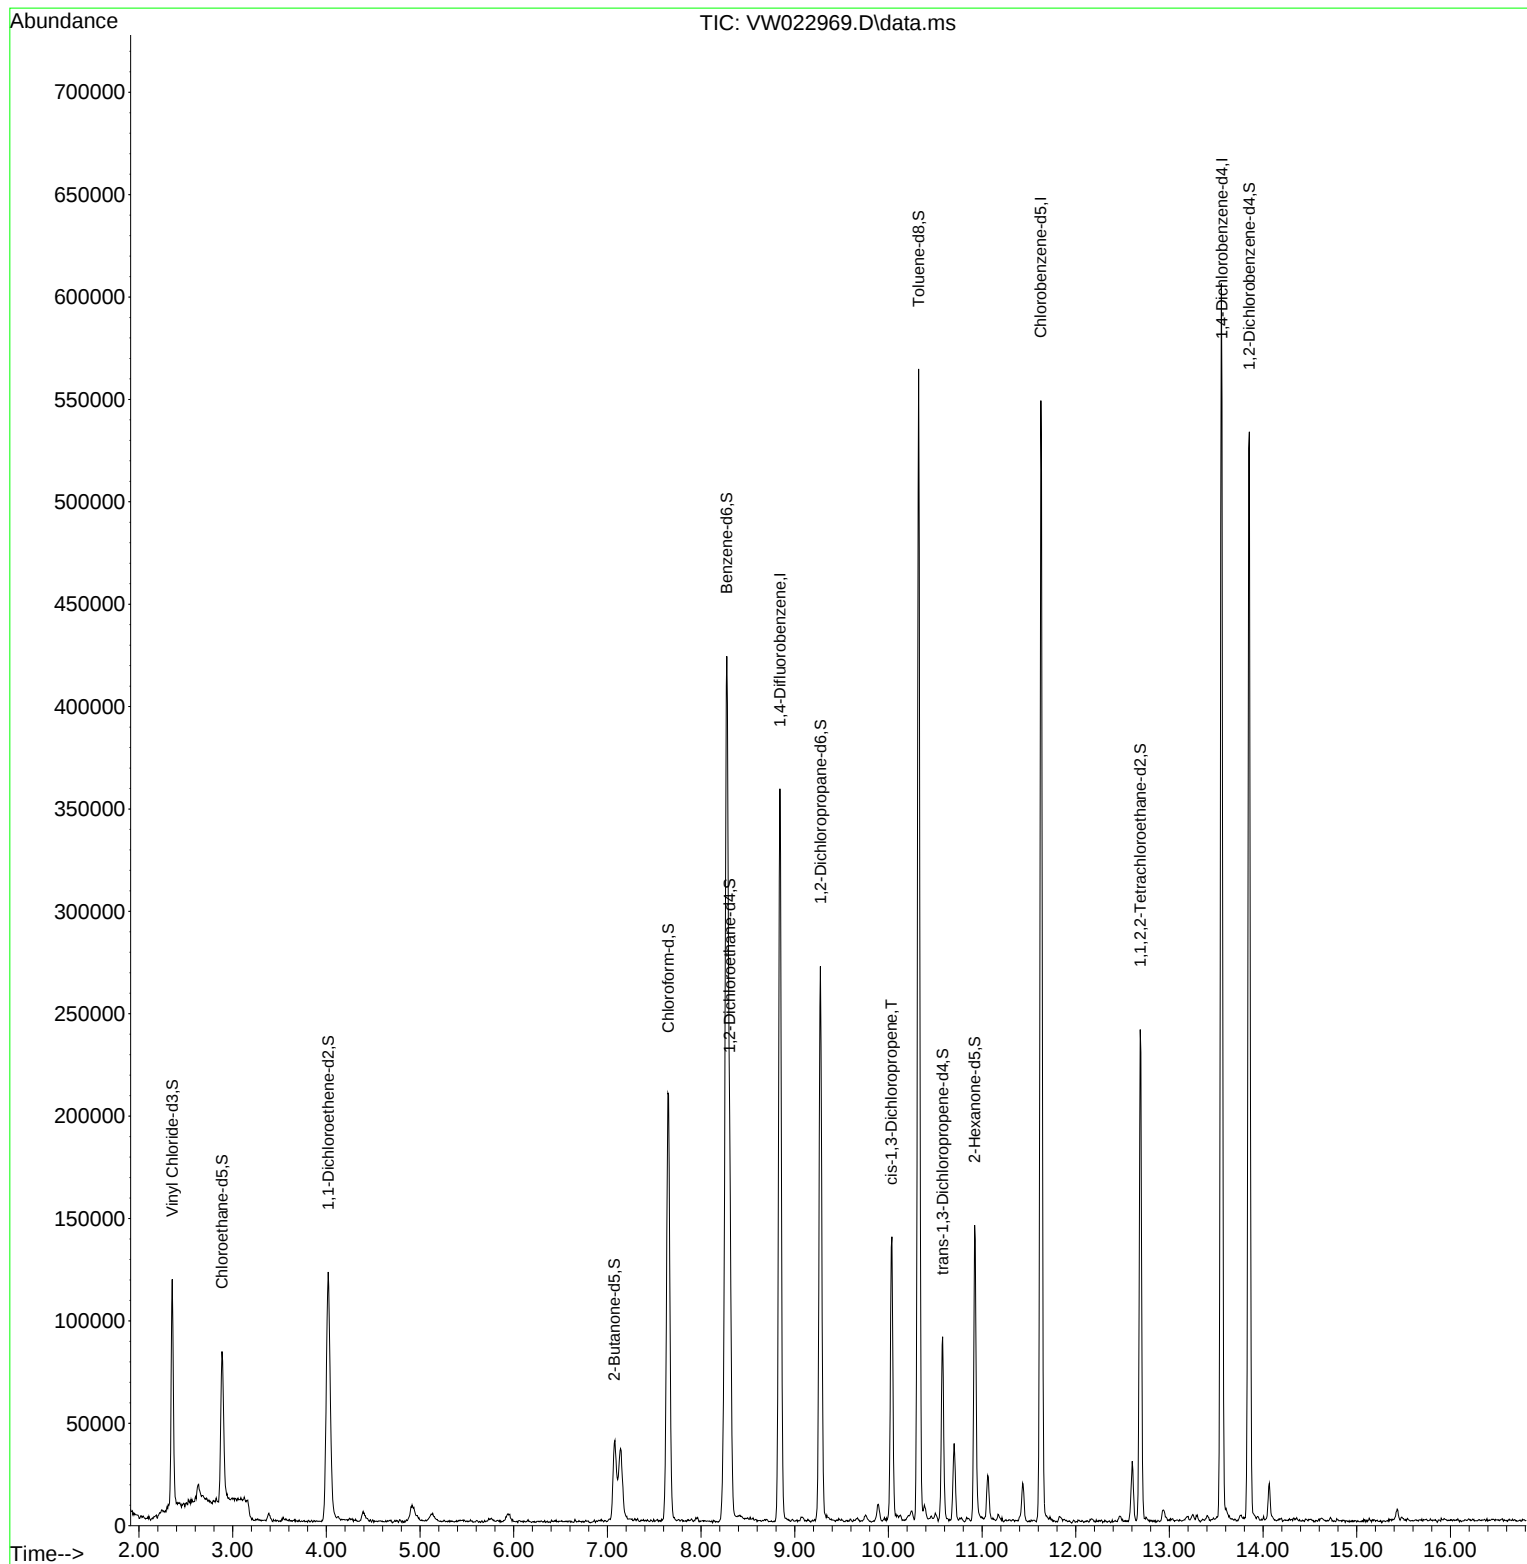

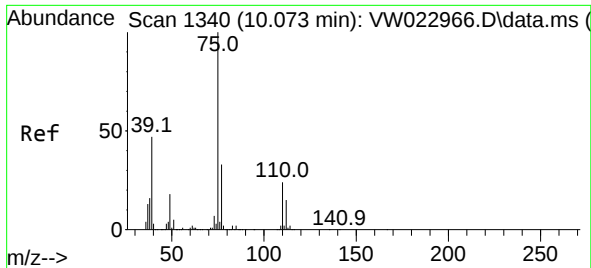

#39
 cis-1,3-Dichloropropene
 Concen: 0.669 ug/L
 RT: 10.031 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VW022969.D
 Acq: 11 May 2022 10:30

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 4385
 Ion Ratio Lower Upper
 75 100
 77 38.2 22.1 41.1

