

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
 Data File : VW022973.D
 Acq On : 11 May 2022 12:05
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK459

Quant Time: May 12 01:10:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 12 01:07:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	303577	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	301027	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	152289	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	105104	16.875	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.520%
7) Chloroethane-d5	2.892	69	85416	21.080	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.320%
11) 1,1-Dichloroethene-d2	4.019	63	116422	14.466	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.880%
21) 2-Butanone-d5	7.074	46	66318	56.002	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.000%
24) Chloroform-d	7.647	84	210974	23.721	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.880%
26) 1,2-Dichloroethane-d4	8.305	65	121064	24.818	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.280%
32) Benzene-d6	8.275	84	392383	22.614	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.440%
36) 1,2-Dichloropropane-d6	9.275	67	119520	24.522	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.080%
41) Toluene-d8	10.323	98	369493	22.045	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.160%
43) trans-1,3-Dichloroprop...	10.579	79	50190	22.365	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.440%
47) 2-Hexanone-d5	10.921	63	52362	56.277	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.560%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	121230	26.686	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	131724	24.744	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.960%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4919	0.739	ug/L	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
Data File : VW022973.D
Acq On : 11 May 2022 12:05
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK459

Quant Time: May 12 01:10:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 12 01:07:03 2022
Response via : Initial Calibration

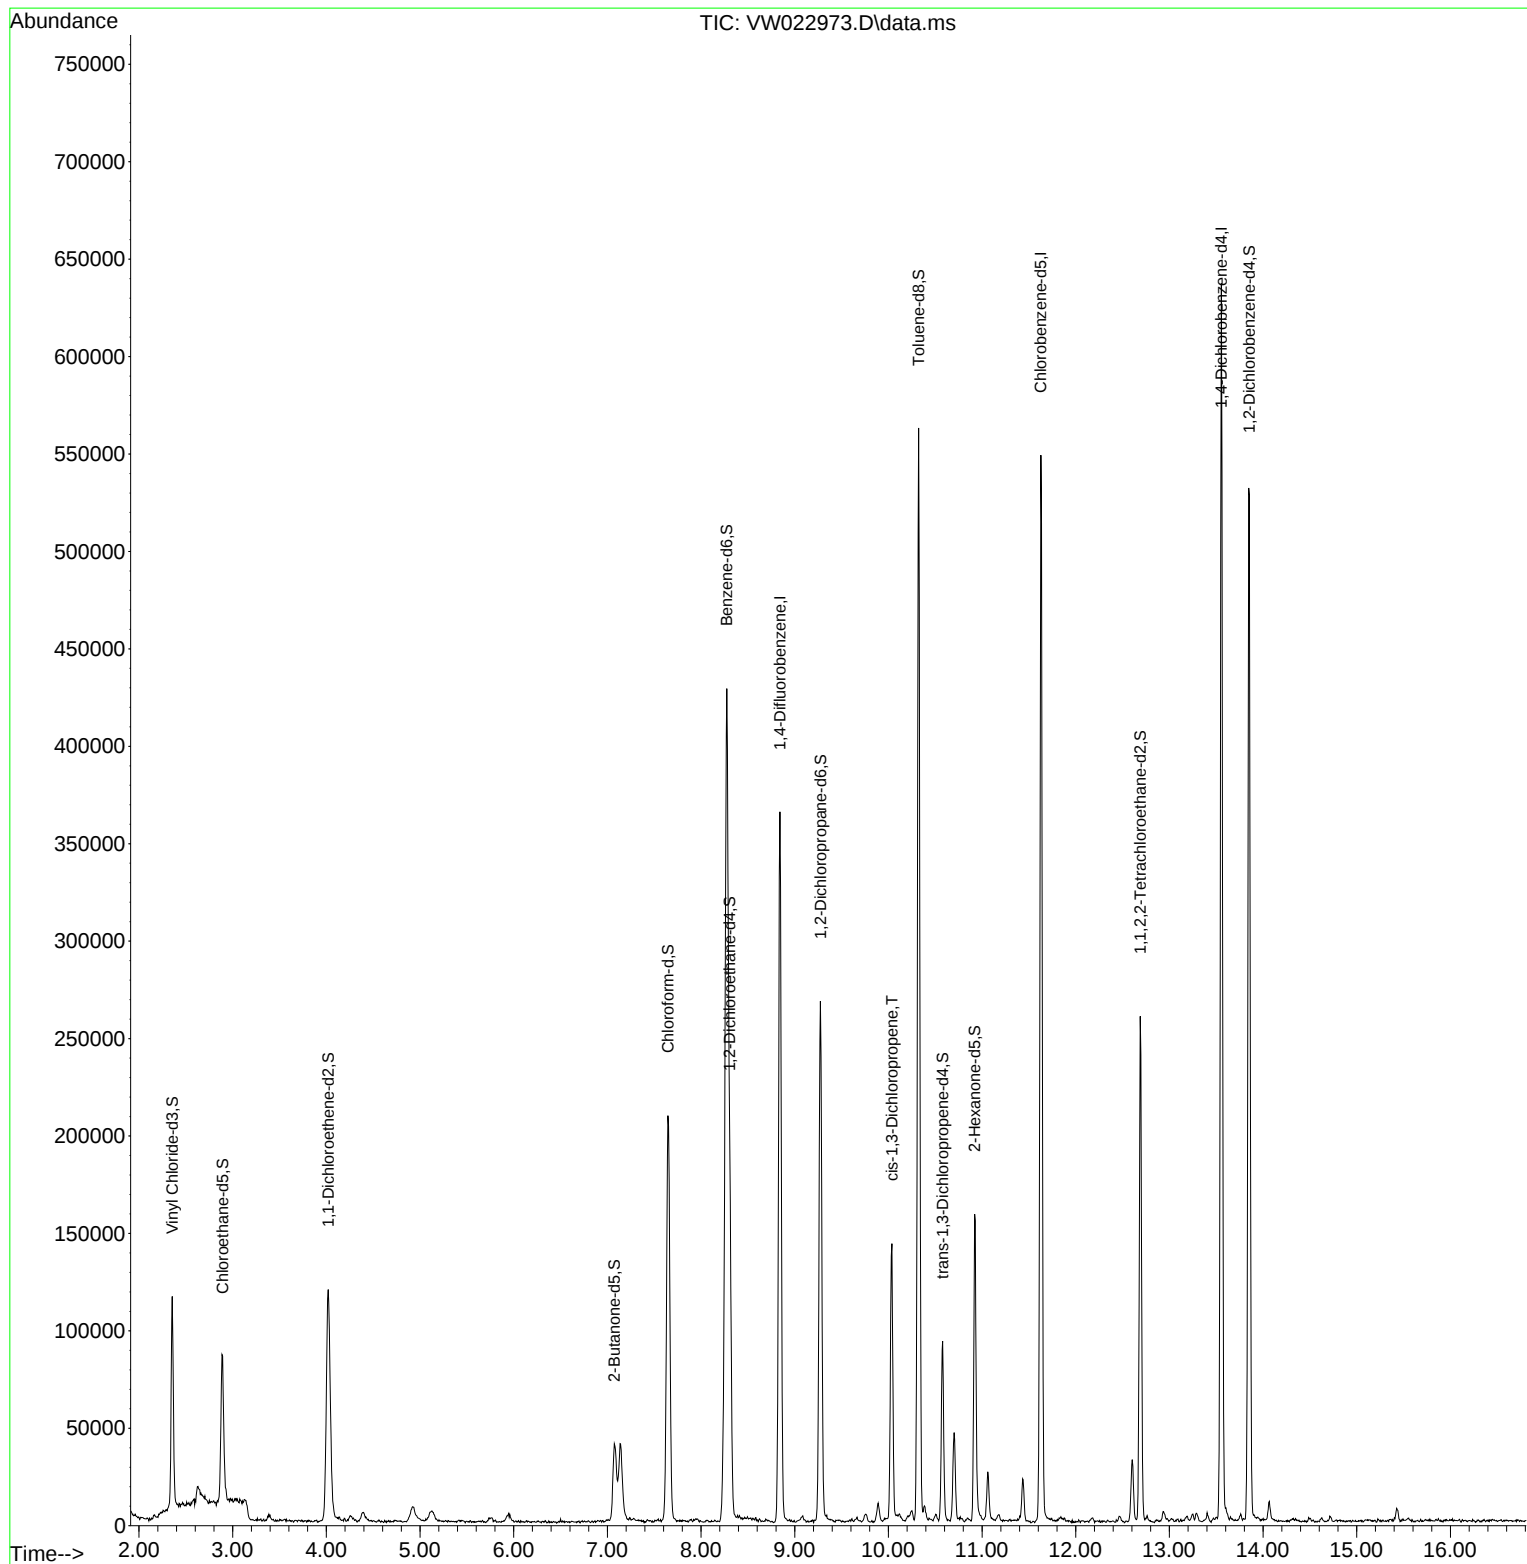

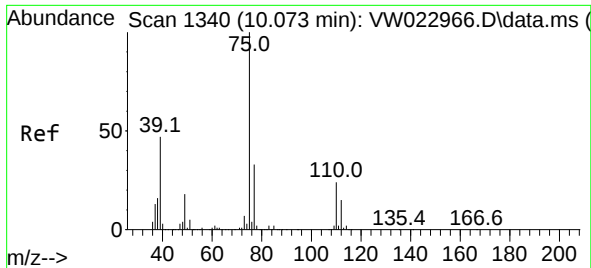

#39
 cis-1,3-Dichloropropene
 Concen: 0.739 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022973.D
 Acq: 11 May 2022 12:05

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK459

Tgt Ion: 75 Resp: 4919
 Ion Ratio Lower Upper
 75 100
 77 47.0 22.1 41.1#

