




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
 Data File : VW022979.D
 Acq On : 11 May 2022 14:29
 Operator : SY/VA
 Sample : N2767-04
 Misc : 6.12g/10mL/MSVOA_W/soil
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM7

Manual IntegrationsAPPROVED

Quant Time: May 12 01:11:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 12 01:07:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

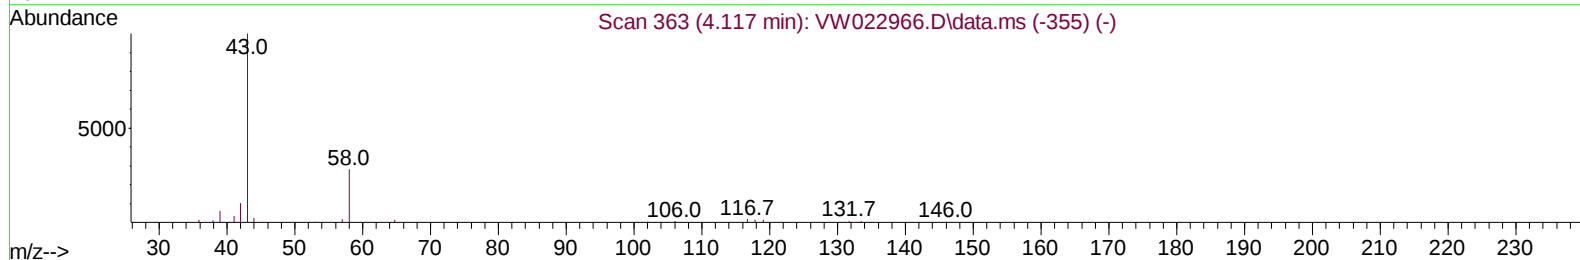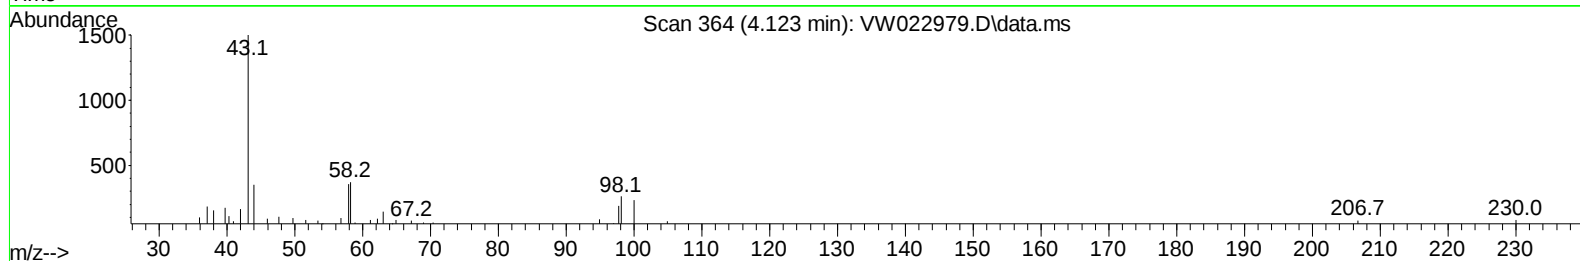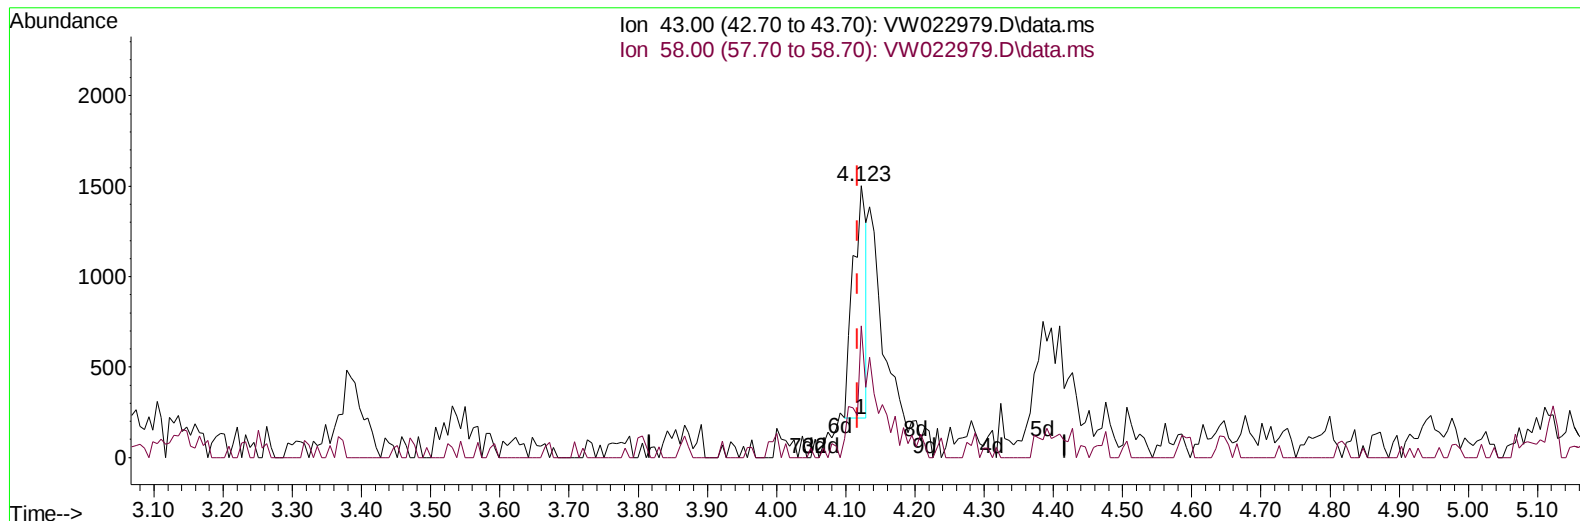

TIC: VW022979.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 2.16 ug/L

response 1685

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	14.07
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
 Data File : VW022979.D
 Acq On : 11 May 2022 14:29
 Operator : SY/VA
 Sample : N2767-04
 Misc : 6.12g/10mL/MSVOA_W/soil
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM7

Manual IntegrationsAPPROVED

Quant Time: May 12 01:11:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 12 01:07:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

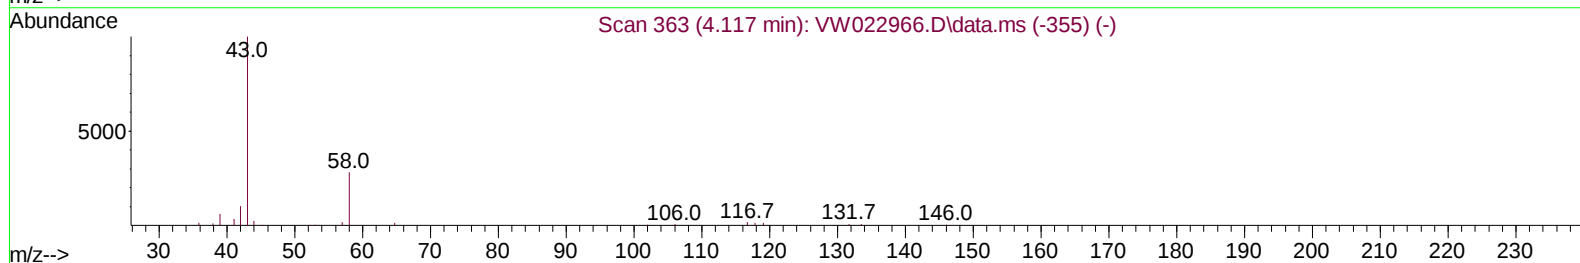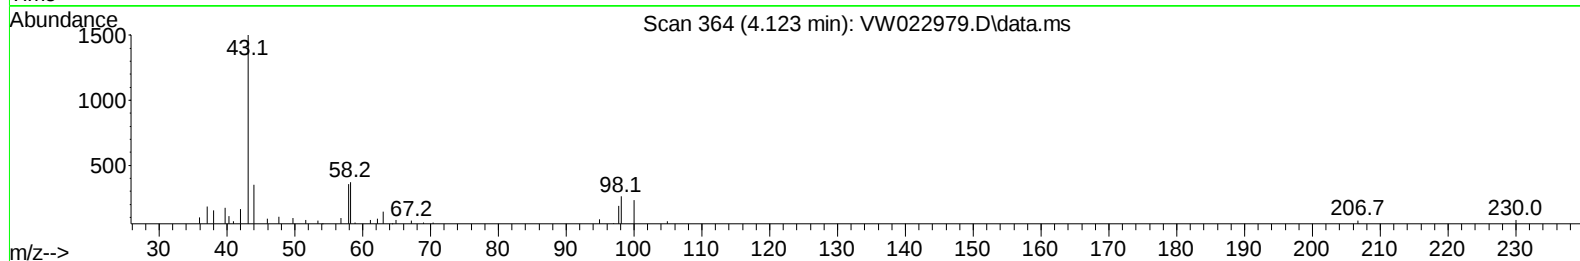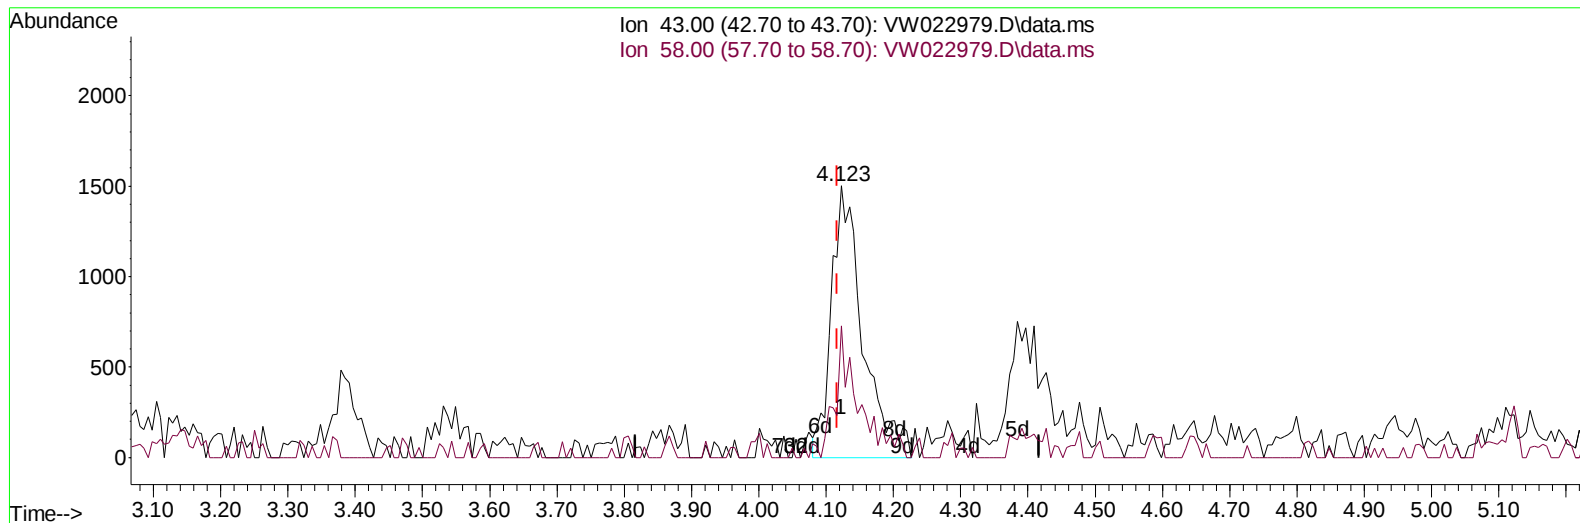

TIC: VW022979.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 6.25 ug/L m

response 4890

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	4.85
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
 Data File : VW022979.D
 Acq On : 11 May 2022 14:29
 Operator : SY/VA
 Sample : N2767-04
 Misc : 6.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM7

Manual IntegrationsAPPROVED

Quant Time: May 12 01:11:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 12 01:07:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	267713	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	205736	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	57200	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	103289	18.805	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.240%	
7) Chloroethane-d5	2.885	69	85893	24.037	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	96.160%	
11) 1,1-Dichloroethene-d2	4.019	63	103902	14.640	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	58.560%	
21) 2-Butanone-d5	7.073	46	62656	59.998	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.000%	
24) Chloroform-d	7.652	84	201454	25.685	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	102.720%	
26) 1,2-Dichloroethane-d4	8.305	65	114710	26.666	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	106.680%	
32) Benzene-d6	8.274	84	341576	28.804	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	115.200%	
36) 1,2-Dichloropropane-d6	9.274	67	111842	33.575	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	134.320%#	
41) Toluene-d8	10.323	98	278137	24.280	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	97.120%	
43) trans-1,3-Dichloroprop...	10.579	79	40313	26.284	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	105.120%	
47) 2-Hexanone-d5	10.920	63	47560	74.792	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	149.580%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	92032	29.642	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	118.560%	
66) 1,2-Dichlorobenzene-d4	13.853	152	49252	24.632	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	98.520%	
Target Compounds						
						Qvalue
13) Acetone	4.123	43	4890m	6.254	ug/L	
46) Tetrachloroethene	10.859	164	43677	17.437	ug/L	82
52) Ethylbenzene	11.731	91	41046	2.716	ug/L	96
53) m,p-Xylene	11.835	106	67704	11.371	ug/L	98
54) o-Xylene	12.164	106	20558	3.598	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
Data File : VW022979.D
Acq On : 11 May 2022 14:29
Operator : SY/VA
Sample : N2767-04
Misc : 6.12g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGPM7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 12 01:11:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 12 01:07:03 2022
Response via : Initial Calibration

