

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
 Data File : VW022974.D
 Acq On : 11 May 2022 12:29
 Operator : SY/VA
 Sample : N2766-04RE
 Misc : 7.09g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4F4RE

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2022
 Supervised By : Mahesh Dadoda 05/16/2022

Quant Time: May 12 01:10:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 12 01:07:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	280128	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	186032	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	39651	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	104669	18.212	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.840%
7) Chloroethane-d5	2.885	69	87414	23.379	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.520%
11) 1,1-Dichloroethene-d2	4.013	63	109252m	14.712	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.840%
21) 2-Butanone-d5	7.086	46	54890	50.232	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.460%
24) Chloroform-d	7.653	84	196255	23.913	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.640%
26) 1,2-Dichloroethane-d4	8.305	65	103244	22.937	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.760%
32) Benzene-d6	8.275	84	345335	32.206	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	128.840%
36) 1,2-Dichloropropane-d6	9.274	67	107742	35.770	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	143.080%#
41) Toluene-d8	10.323	98	261342	25.230	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.920%
43) trans-1,3-Dichloroprop...	10.579	79	29905	21.563	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.240%
47) 2-Hexanone-d5	10.927	63	38639	67.199	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.400%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	88084	31.375	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	125.520%#
66) 1,2-Dichlorobenzene-d4	13.847	152	41910	30.237	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	120.960%#
Target Compounds					Qvalue	
13) Acetone	4.141	43	5315	6.497	ug/L	52

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
Data File : VW022974.D
Acq On : 11 May 2022 12:29
Operator : SY/VA
Sample : N2766-04RE
Misc : 7.09g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW4F4RE

Quant Time: May 12 01:10:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 12 01:07:03 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

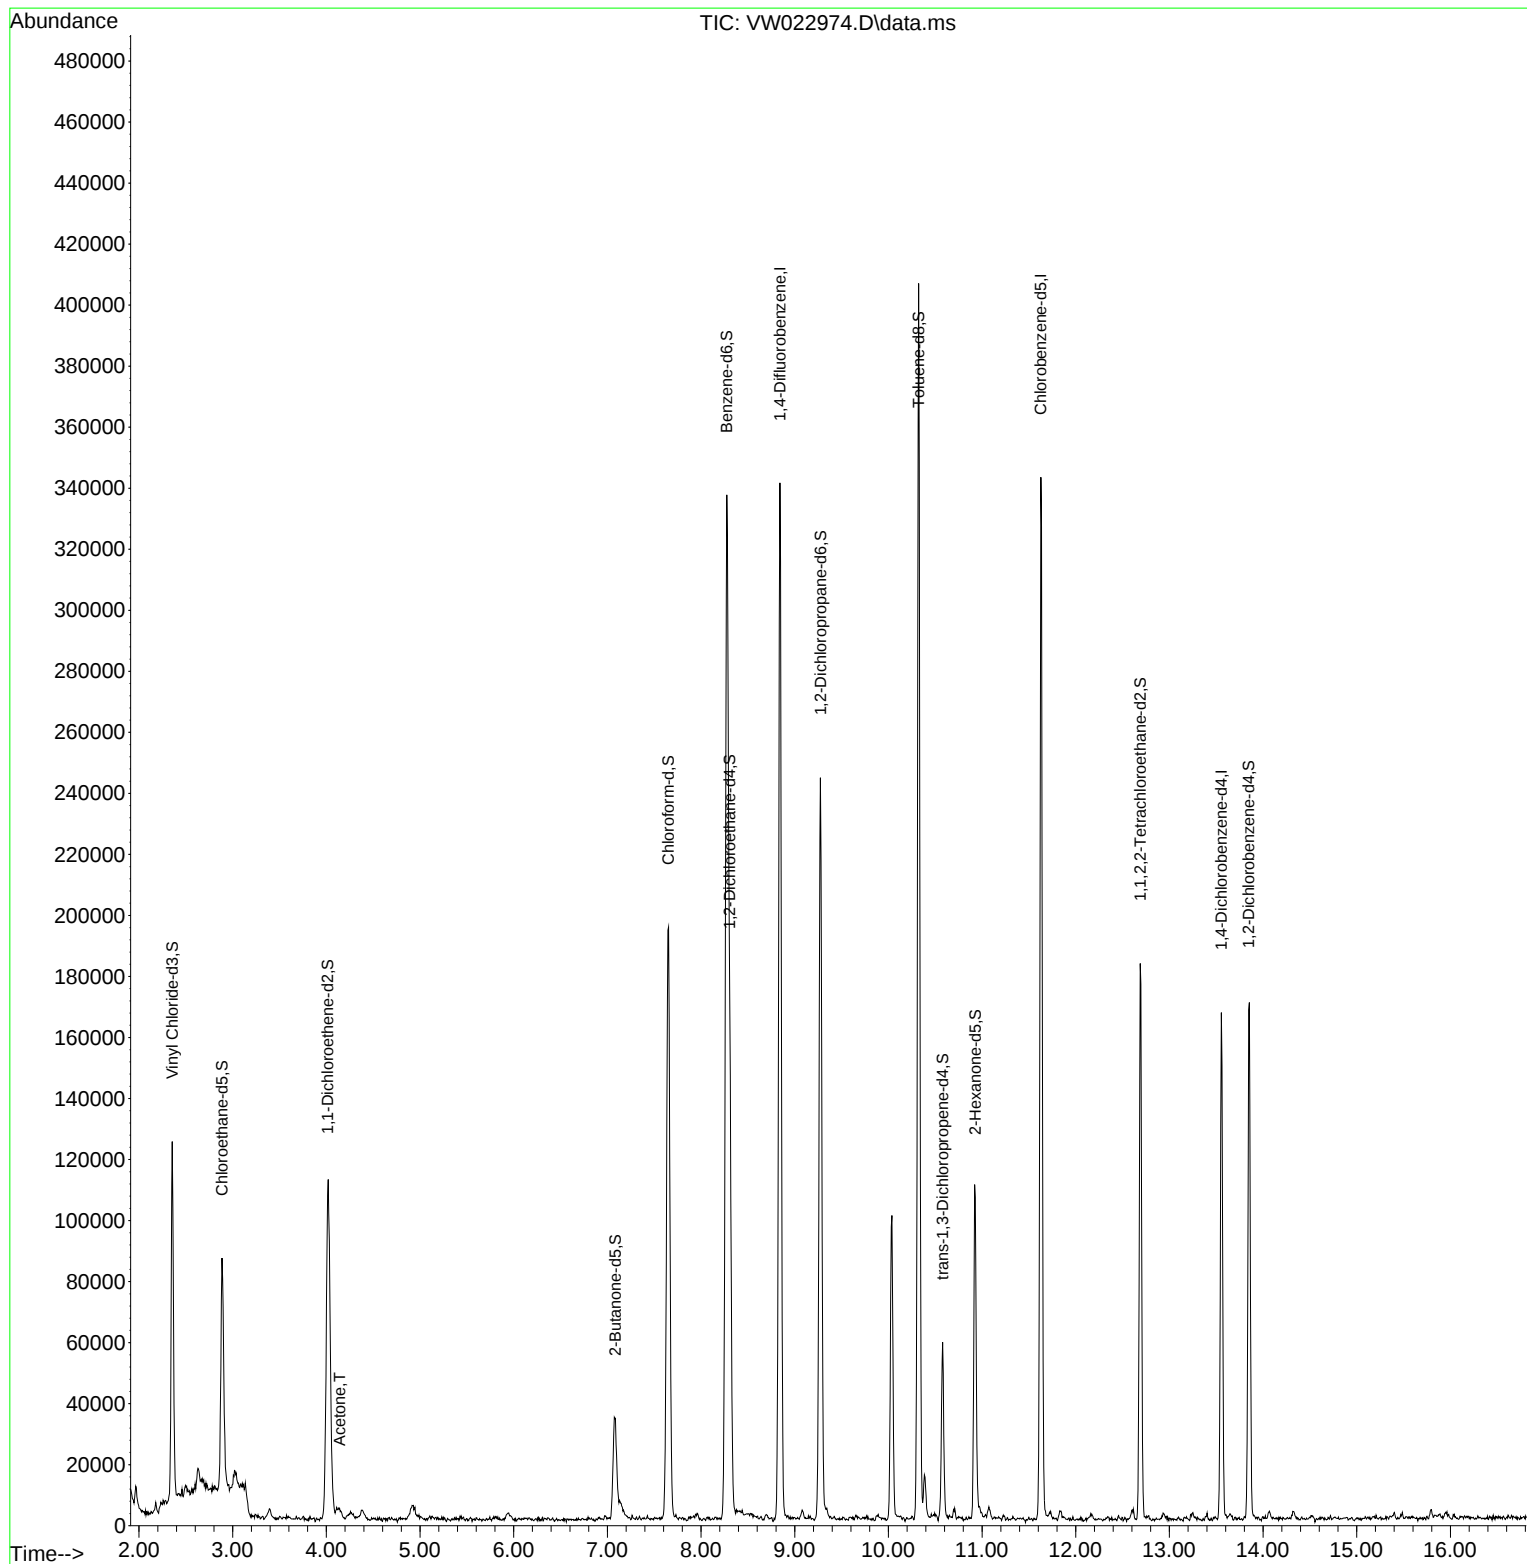

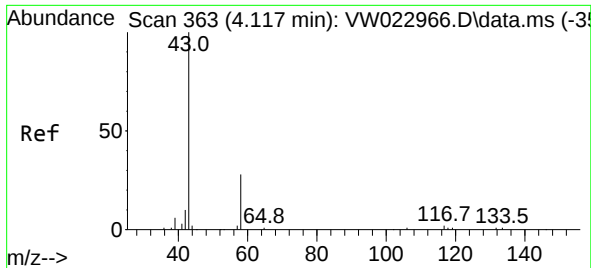

#13

Acetone

Concen: 6.497 ug/L

RT: 4.141 min Scan# 30

Delta R.T. 0.024 min

Lab File: VW022974.D

Acq: 11 May 2022 12:29

Instrument :

MSVOA_W

ClientSampleId :

EW4F4RE

Tgt Ion: 43 Resp: 531

Ion Ratio Lower Upper

43 100

58 5.2 0.0 64.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022

Supervised By :Mahesh Dadoda 05/16/2022

