

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
 Data File : VW022977.D
 Acq On : 11 May 2022 13:41
 Operator : SY/VA
 Sample : N2767-02
 Misc : 4.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPL9

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2022
 Supervised By : Mahesh Dadoda 05/16/2022

Quant Time: May 12 01:11:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 12 01:07:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	345913	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	331202	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	163712	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	109696	15.457	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	61.840%		
7) Chloroethane-d5	2.891	69	92590	20.054	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.200%		
11) 1,1-Dichloroethene-d2	4.019	63	124453	13.572	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	54.280%		
21) 2-Butanone-d5	7.080	46	63065	46.737	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.480%		
24) Chloroform-d	7.647	84	225175	22.219	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.880%		
26) 1,2-Dichloroethane-d4	8.305	65	125838m	22.639	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.560%		
32) Benzene-d6	8.275	84	408290	21.387	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.560%		
36) 1,2-Dichloropropane-d6	9.274	67	126803	23.646	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.600%		
41) Toluene-d8	10.323	98	380119	20.612	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.440%		
43) trans-1,3-Dichloroprop...	10.579	79	50545	20.471	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.880%		
47) 2-Hexanone-d5	10.920	63	51143	49.959	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	99.920%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	120284	24.065	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	96.280%		
66) 1,2-Dichlorobenzene-d4	13.853	152	131647	23.004	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.000%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	5513	5.457	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051122\
Data File : VW022977.D
Acq On : 11 May 2022 13:41
Operator : SY/VA
Sample : N2767-02
Misc : 4.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BGPL9

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/15/2022
Supervised By : Mahesh Dadoda 05/16/2022

Quant Time: May 12 01:11:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 12 01:07:03 2022
Response via : Initial Calibration

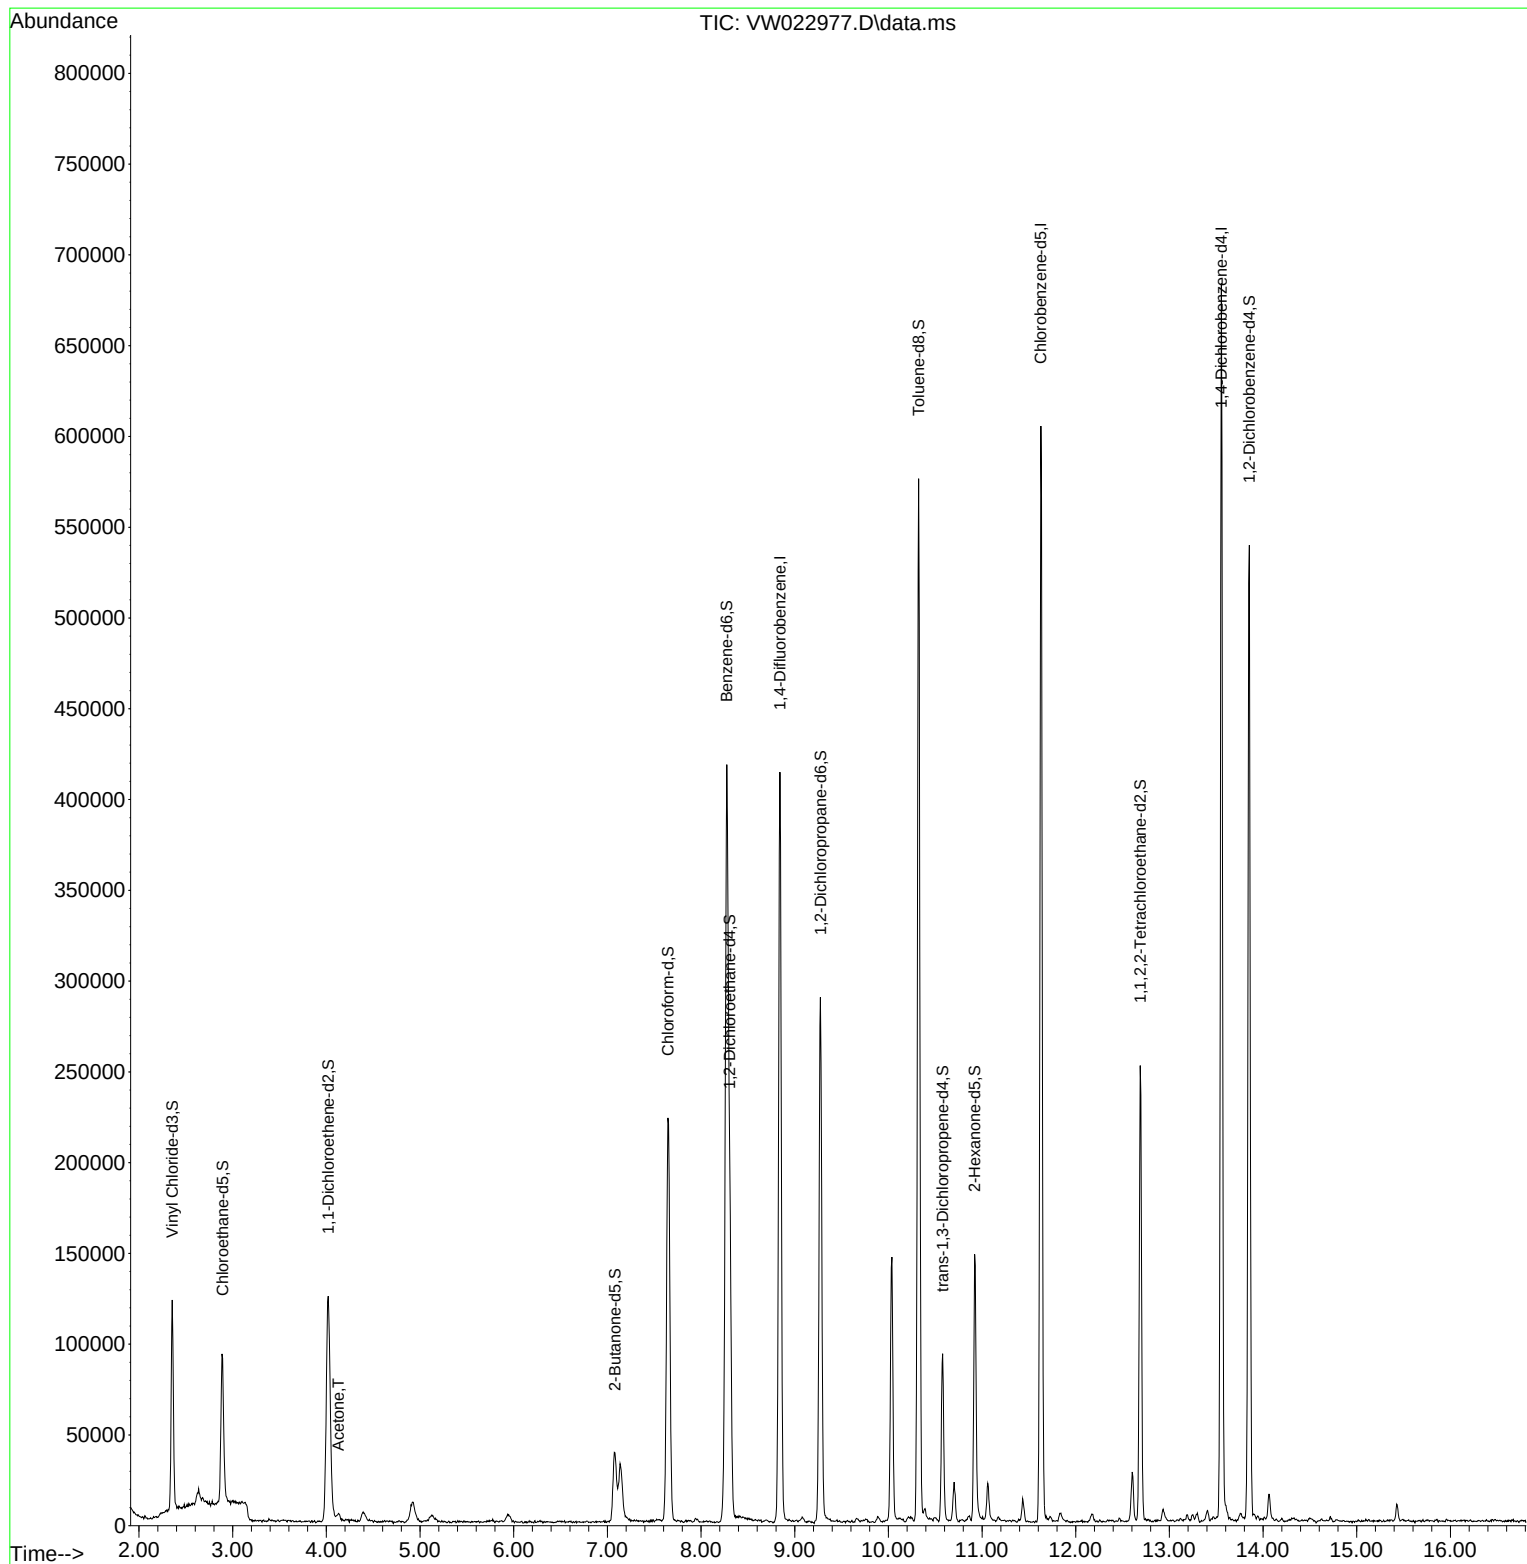

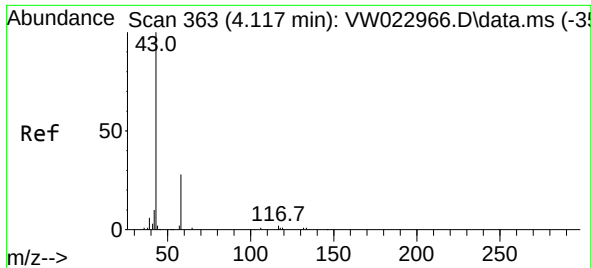

#13
 Acetone
 Concen: 5.457 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW022977.D
 Acq: 11 May 2022 13:41

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPL9

Tgt Ion: 43 Resp: 551
 Ion Ratio Lower Upper
 43 100
 58 28.6 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

