

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW022994.D
 Acq On : 12 May 2022 11:42
 Operator : SY/VA
 Sample : N2766-10
 Misc : 7.65g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4G0

Quant Time: May 13 01:11:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	278154	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	245630	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93662	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	83960	14.712	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.840%
7) Chloroethane-d5	2.891	69	68765	18.522	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.080%
11) 1,1-Dichloroethene-d2	4.019	63	86336	11.709	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.840%
21) 2-Butanone-d5	7.080	46	50428	46.476	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.960%
24) Chloroform-d	7.653	84	164936	20.239	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.960%
26) 1,2-Dichloroethane-d4	8.305	65	95021	21.260	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.040%
32) Benzene-d6	8.275	84	293106	20.703	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.800%
36) 1,2-Dichloropropane-d6	9.274	67	92891	23.357	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.440%
41) Toluene-d8	10.323	98	252538	18.465	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.840%
43) trans-1,3-Dichloroprop...	10.579	79	33279	18.174	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.680%
47) 2-Hexanone-d5	10.920	63	40357	53.157	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.320%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	87528	23.613	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	68370	20.882	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.520%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	3319	0.611	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
Data File : VW022994.D
Acq On : 12 May 2022 11:42
Operator : SY/VA
Sample : N2766-10
Misc : 7.65g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4G0

Quant Time: May 13 01:11:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 01:10:05 2022
Response via : Initial Calibration

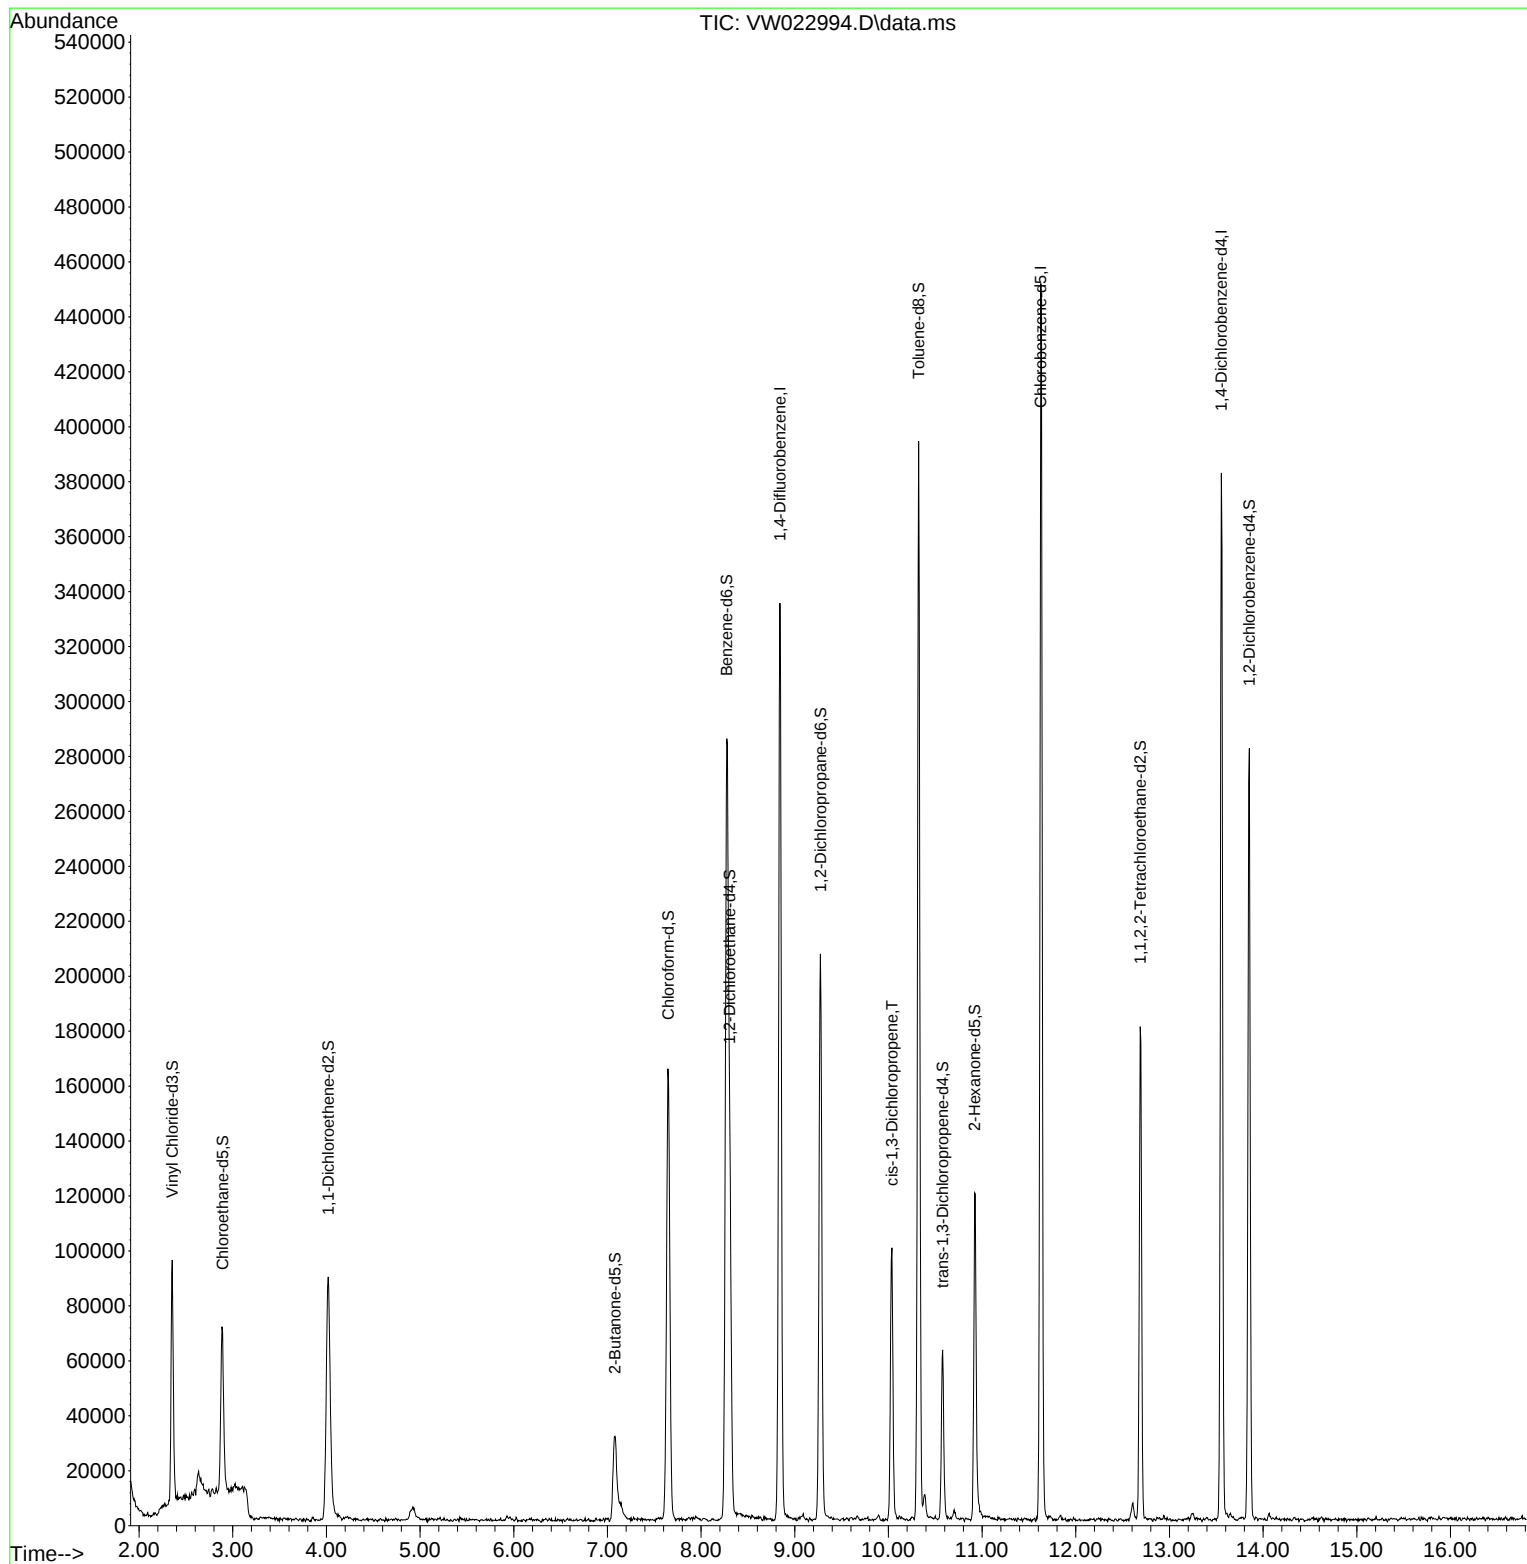

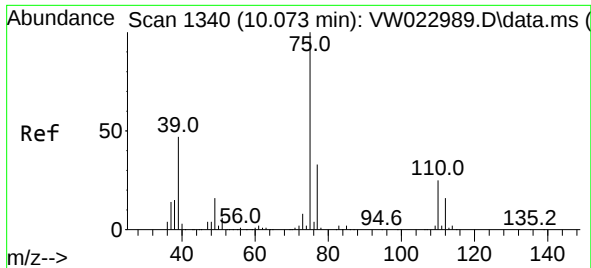

#39
 cis-1,3-Dichloropropene
 Concen: 0.611 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022994.D
 Acq: 12 May 2022 11:42

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4G0

Tgt Ion: 75 Resp: 3319
 Ion Ratio Lower Upper
 75 100
 77 47.4 22.1 41.1#

