

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW022997.D
 Acq On : 12 May 2022 13:19
 Operator : SY/VA
 Sample : N2766-11RE
 Misc : 5.32g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4G1RE

Quant Time: May 13 01:11:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	298742	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	233660	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	59537	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	94220	15.372	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.480%
7) Chloroethane-d5	2.885	69	74419	18.663	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.640%
11) 1,1-Dichloroethene-d2	4.019	63	97541	12.317	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.280%
21) 2-Butanone-d5	7.073	46	52494	45.046	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.100%
24) Chloroform-d	7.646	84	180084	20.575	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.320%
26) 1,2-Dichloroethane-d4	8.305	65	97774	20.368	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.480%
32) Benzene-d6	8.268	84	321292	23.856	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.440%
36) 1,2-Dichloropropane-d6	9.274	67	99402	26.275	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.080%
41) Toluene-d8	10.323	98	267138	20.533	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.120%
43) trans-1,3-Dichloroprop...	10.573	79	32428	18.616	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.480%
47) 2-Hexanone-d5	10.920	63	37372	51.747	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.500%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	81295	23.055	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	13.853	152	47485	22.816	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.280%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	2936	0.568	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
Data File : VW022997.D
Acq On : 12 May 2022 13:19
Operator : SY/VA
Sample : N2766-11RE
Misc : 5.32g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4G1RE

Quant Time: May 13 01:11:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 01:10:05 2022
Response via : Initial Calibration

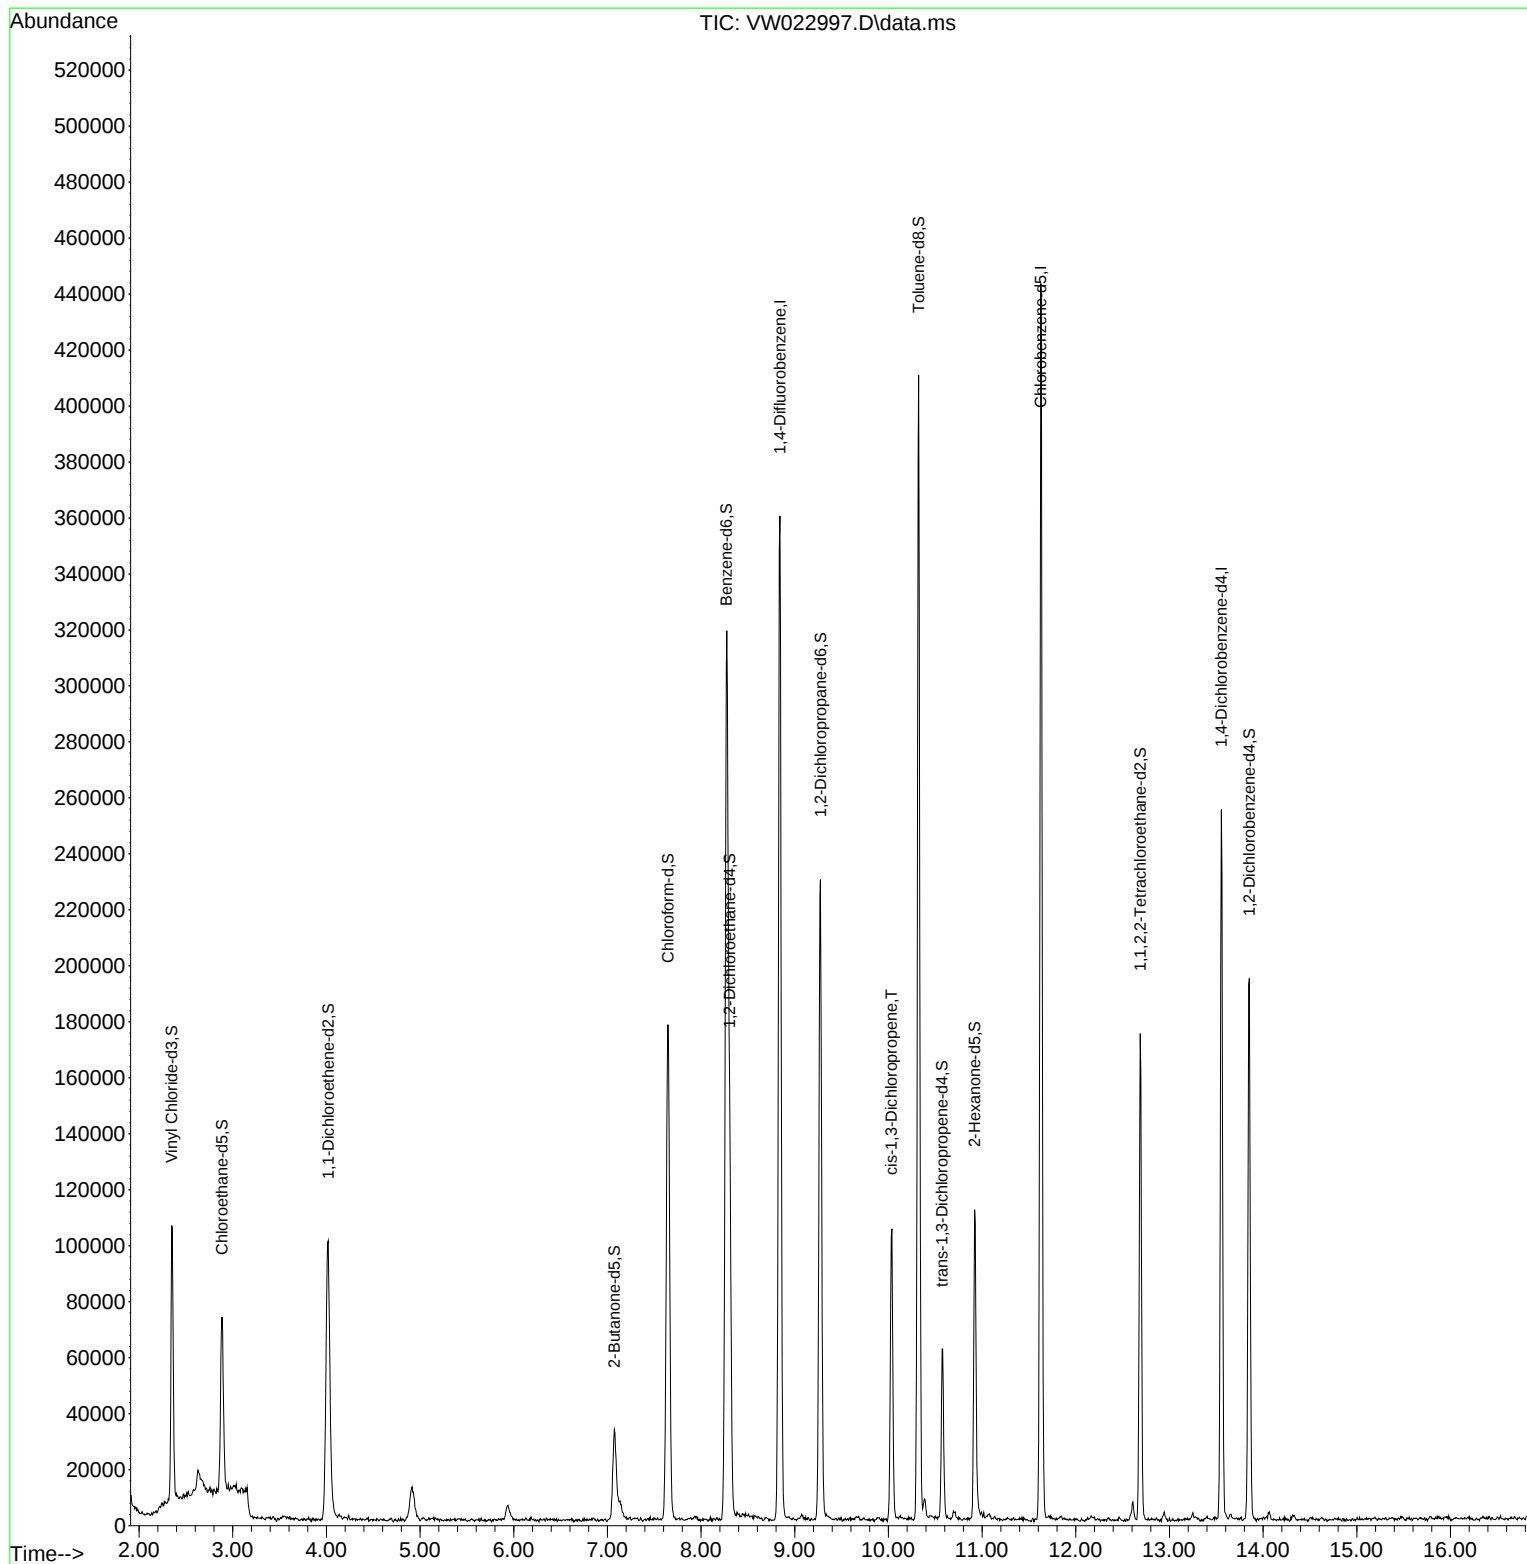

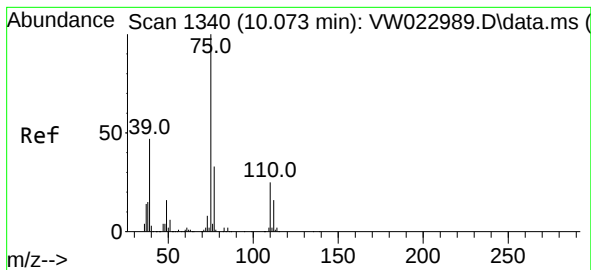

#39
 cis-1,3-Dichloropropene
 Concen: 0.568 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW022997.D
 Acq: 12 May 2022 13:19

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4G1RE

Tgt Ion: 75 Resp: 2936
 Ion Ratio Lower Upper
 75 100
 77 37.8 22.1 41.1

