

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW023004.D
 Acq On : 12 May 2022 16:17
 Operator : SY/VA
 Sample : N2766-14
 Misc : 6.74g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4G4

Quant Time: May 13 01:13:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	319953	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	296257	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	120731	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	108500	16.529	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.120%
7) Chloroethane-d5	2.879	69	85331	19.981	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.920%
11) 1,1-Dichloroethene-d2	4.013	63	104732	12.348	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.400%
21) 2-Butanone-d5	7.080	46	49038	39.291	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.580%
24) Chloroform-d	7.647	84	203186	21.676	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.720%
26) 1,2-Dichloroethane-d4	8.305	65	108508	21.106	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.440%
32) Benzene-d6	8.275	84	366137	21.442	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.760%
36) 1,2-Dichloropropane-d6	9.275	67	114402	23.850	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.400%
41) Toluene-d8	10.323	98	328030	19.886	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.560%
43) trans-1,3-Dichloroprop...	10.579	79	40663	18.411	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.640%
47) 2-Hexanone-d5	10.921	63	39100	42.700	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.400%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	94174	21.064	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	91057	21.576	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.320%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.031	75	4129	0.630	ug/L	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
Data File : VW023004.D
Acq On : 12 May 2022 16:17
Operator : SY/VA
Sample : N2766-14
Misc : 6.74g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4G4

Quant Time: May 13 01:13:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 01:10:05 2022
Response via : Initial Calibration

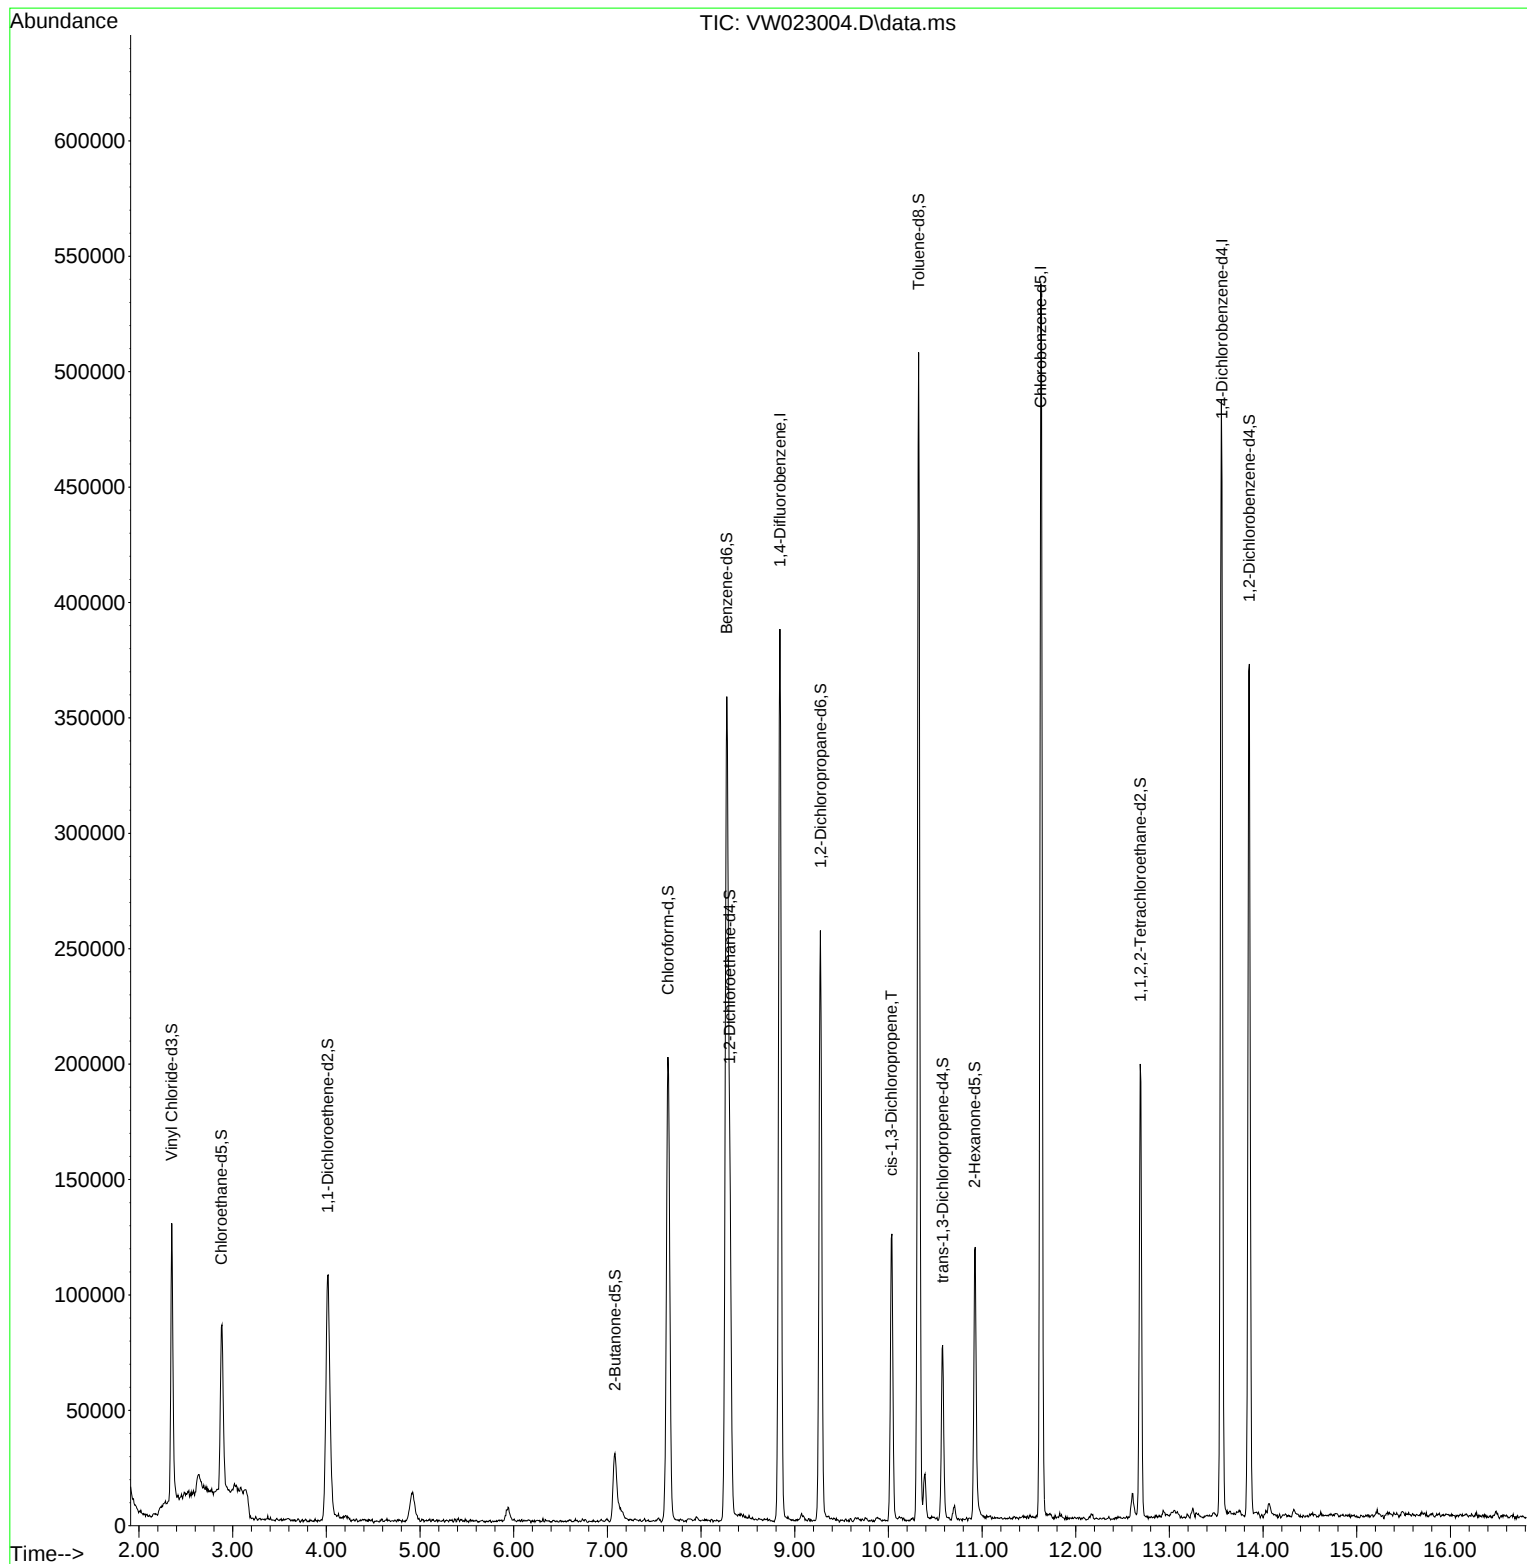

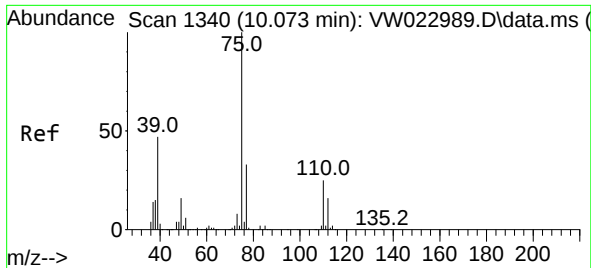

#39

cis-1,3-Dichloropropene

Concen: 0.630 ug/L

RT: 10.031 min Scan# 11

Delta R.T. -0.042 min

Lab File: VW023004.D


Acq: 12 May 2022 16:17

Instrument :

MSVOA_W

ClientSampleId :

EW4G4

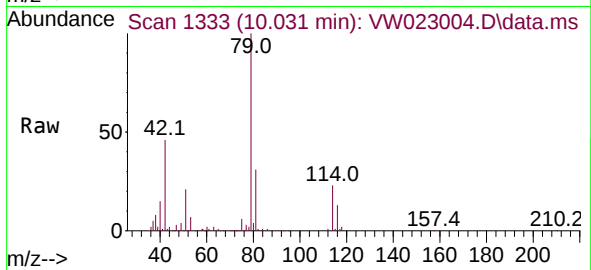

Tgt Ion: 75 Resp: 4129

Ion Ratio Lower Upper

75 100

77 42.5 22.1 41.1#

