




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW022996.D
 Acq On : 12 May 2022 12:30
 Operator : SY/VA
 Sample : N2767-08
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM3

Manual IntegrationsAPPROVED

Quant Time: May 13 01:11:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

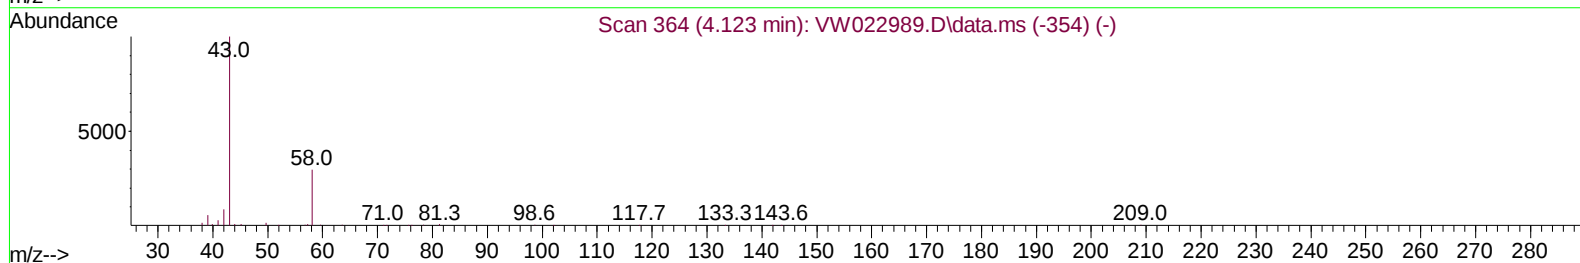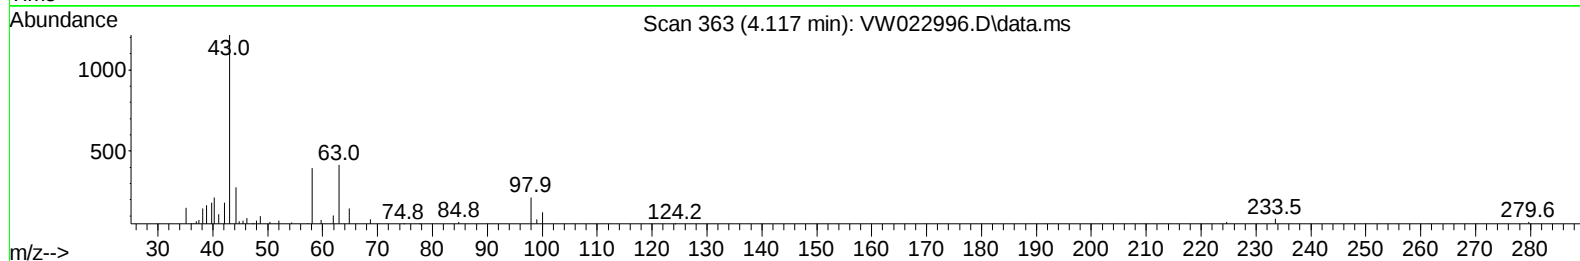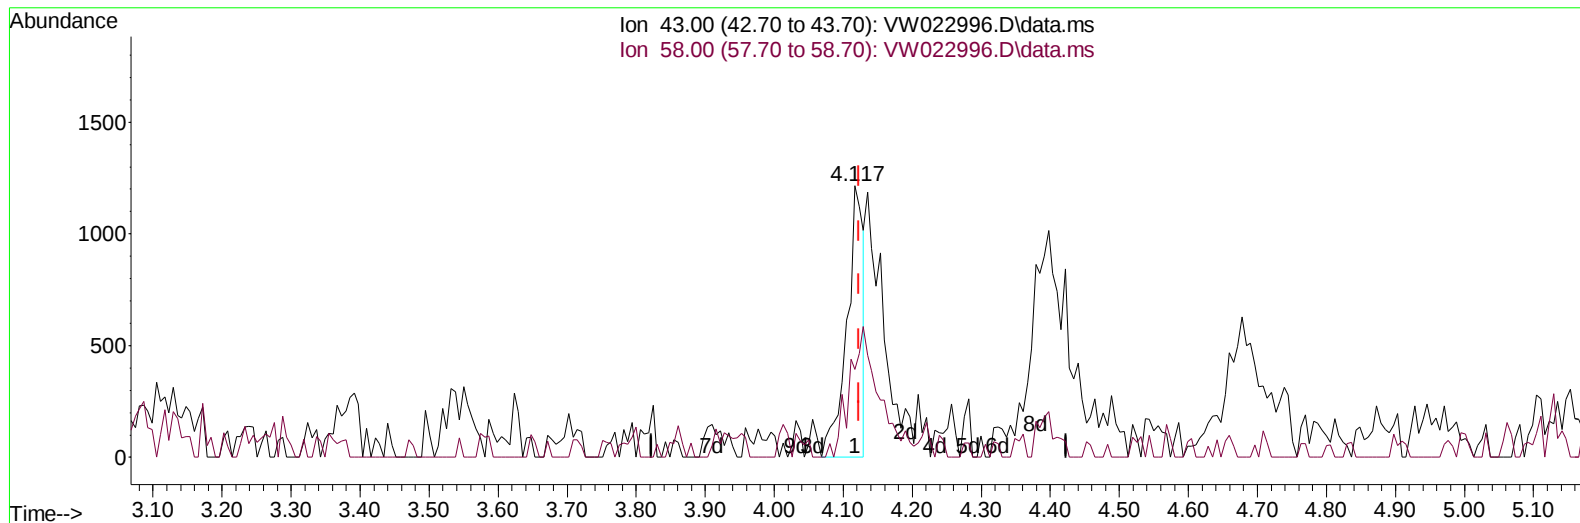

TIC: VW022996.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 2.03 ug/L

response 2034

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	13.62
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW022996.D
 Acq On : 12 May 2022 12:30
 Operator : SY/VA
 Sample : N2767-08
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM3

Manual IntegrationsAPPROVED

Quant Time: May 13 01:11:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

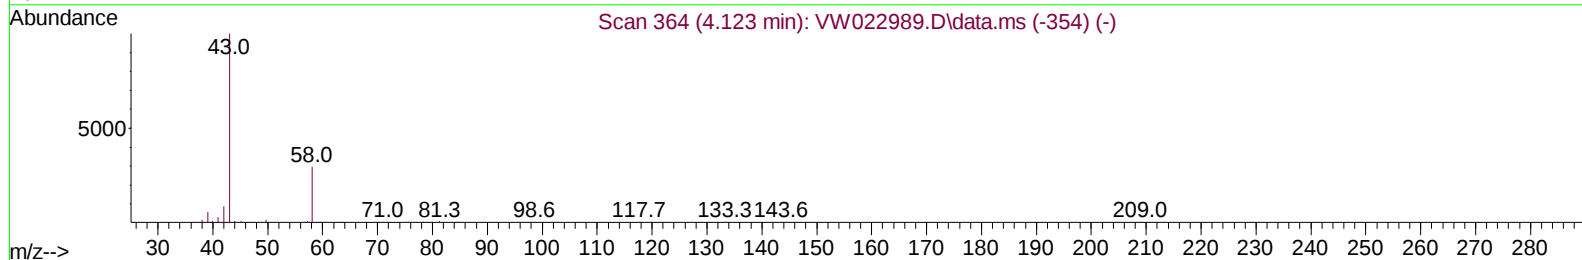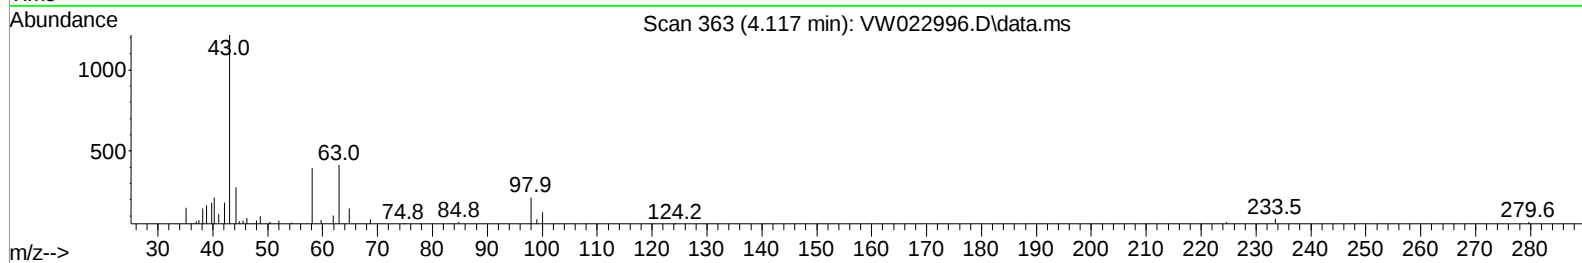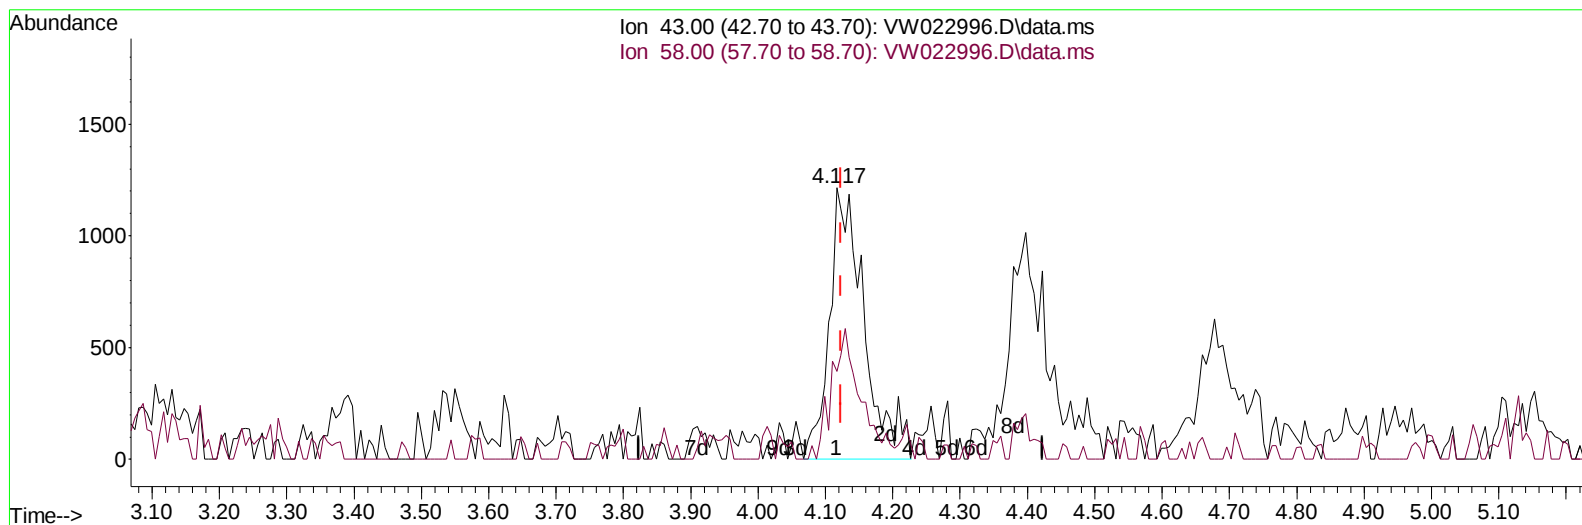

TIC: VW022996.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 4.35 ug/L m

response 4355

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	6.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW022996.D
 Acq On : 12 May 2022 12:30
 Operator : SY/VA
 Sample : N2767-08
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM3

Manual IntegrationsAPPROVED

Quant Time: May 13 01:11:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

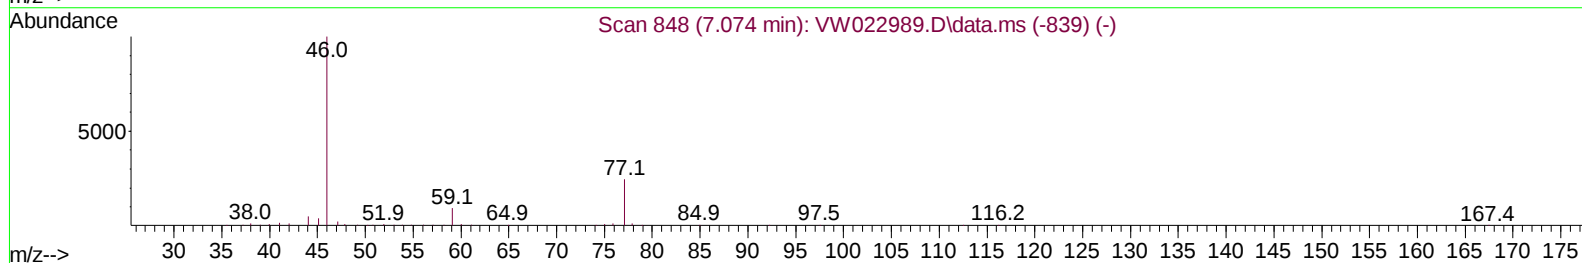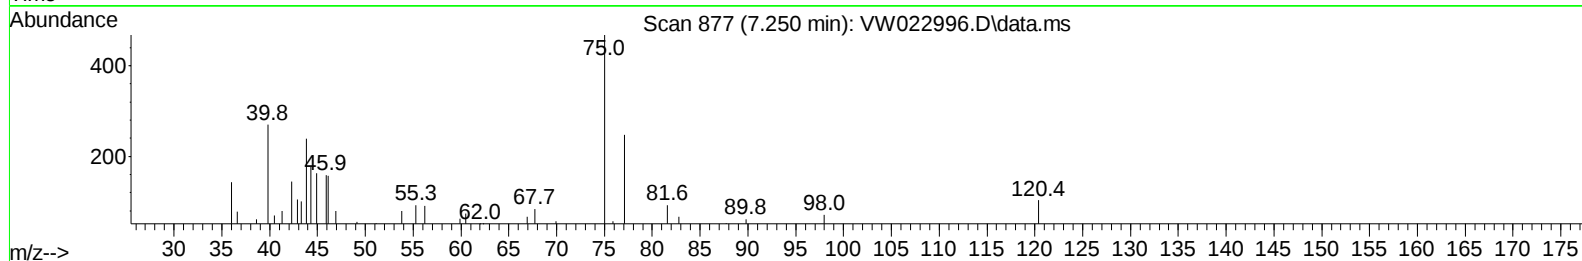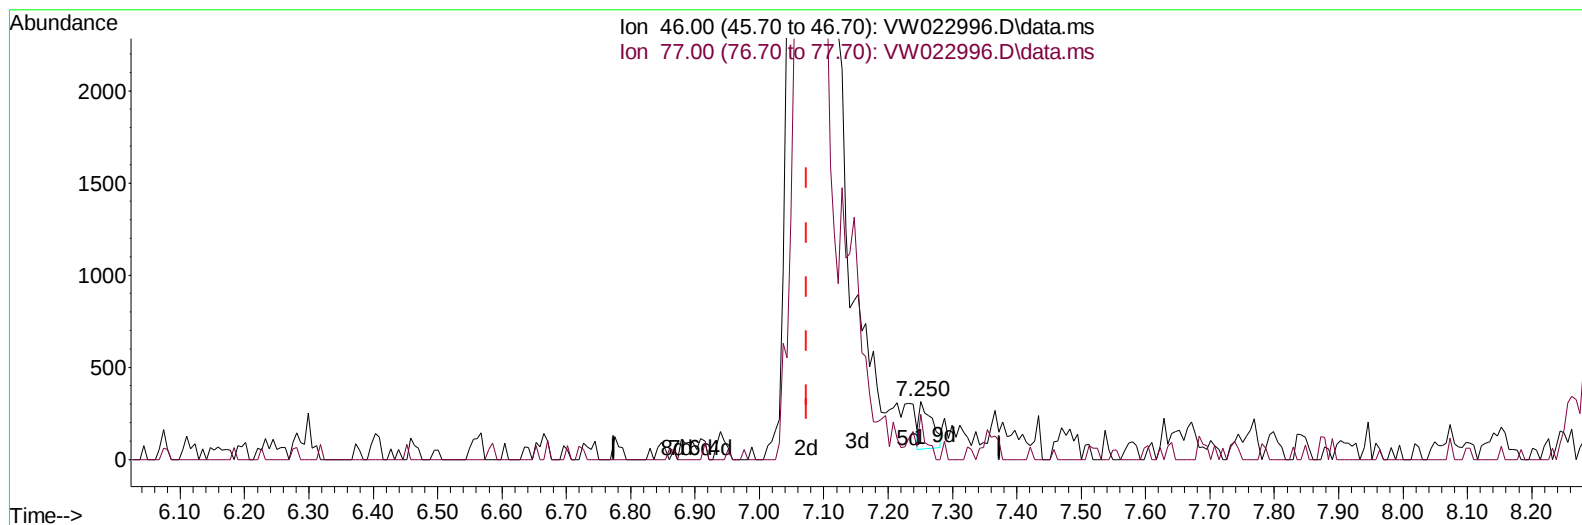

TIC: VW022996.D\data.ms

(21) 2-Butanone-d5 (S)

7.250min (+ 0.177) 0.26 ug/L

response 351

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	21.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW022996.D
 Acq On : 12 May 2022 12:30
 Operator : SY/VA
 Sample : N2767-08
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM3

Manual IntegrationsAPPROVED

Quant Time: May 13 01:11:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

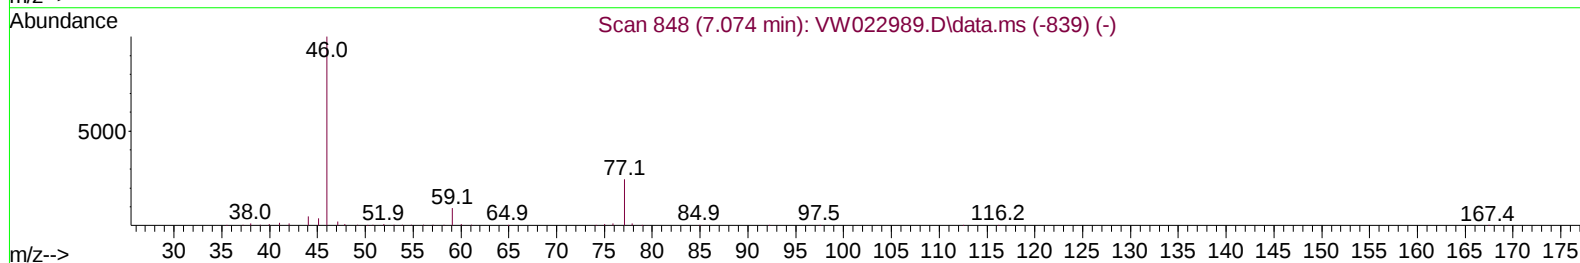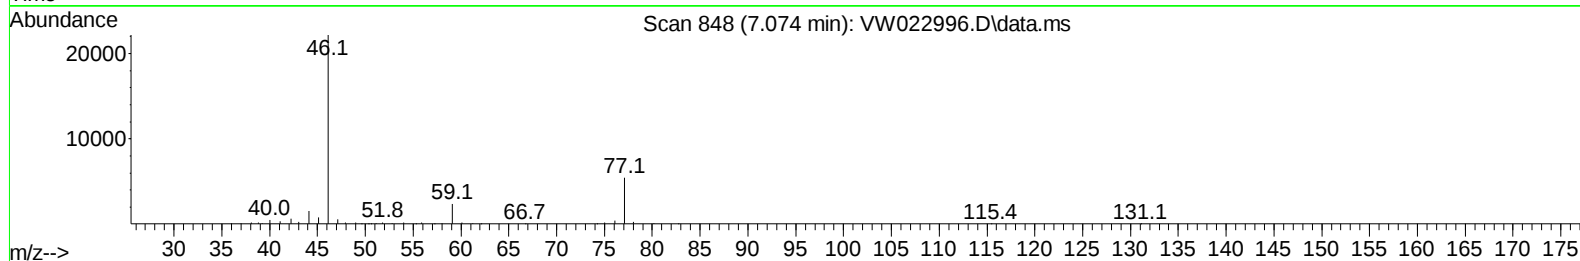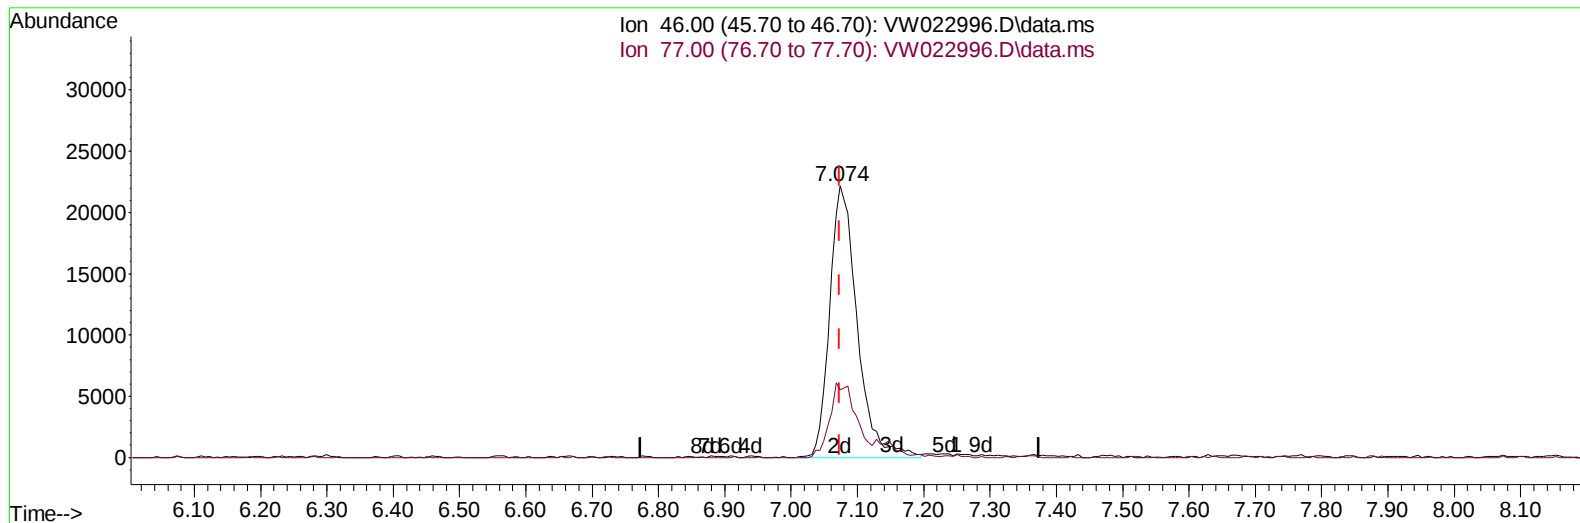

TIC: VW022996.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (+ 0.000) 47.72 ug/L m

response 63768

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.12#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW022996.D
 Acq On : 12 May 2022 12:30
 Operator : SY/VA
 Sample : N2767-08
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 13 01:11:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		342558	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		332101	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		163758	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		98425	14.005	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	56.000%		
7) Chloroethane-d5	2.885	69		86468	18.911	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	75.640%		
11) 1,1-Dichloroethene-d2	4.013	63		107323	11.818	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	47.280%		
21) 2-Butanone-d5	7.074	46		63768m	47.721	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	95.440%		
24) Chloroform-d	7.653	84		207549	20.680	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	82.720%		
26) 1,2-Dichloroethane-d4	8.305	65		119077	21.633	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	86.520%		
32) Benzene-d6	8.275	84		378460	19.771	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	79.080%		
36) 1,2-Dichloropropane-d6	9.274	67		117547	21.861	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	87.440%		
41) Toluene-d8	10.323	98		349817	18.918	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	75.680%		
43) trans-1,3-Dichloroprop...	10.579	79		46624	18.832	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	75.320%		
47) 2-Hexanone-d5	10.921	63		48671	47.416	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	94.840%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		114143	22.775	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	91.080%		
66) 1,2-Dichlorobenzene-d4	13.853	152		121032	21.143	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	84.560%		
Target Compounds							
13) Acetone	4.117	43		4355m	4.353	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
Data File : VW022996.D
Acq On : 12 May 2022 12:30
Operator : SY/VA
Sample : N2767-08
Misc : 5.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGP3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 13 01:11:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 01:10:05 2022
Response via : Initial Calibration

