




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
Data File : VW023007.D
Acq On : 12 May 2022 17:29
Operator : SY/VA
Sample : N2766-17
Misc : 6.88g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4G7

Manual IntegrationsAPPROVED

Quant Time: May 13 01:13:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 01:10:05 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

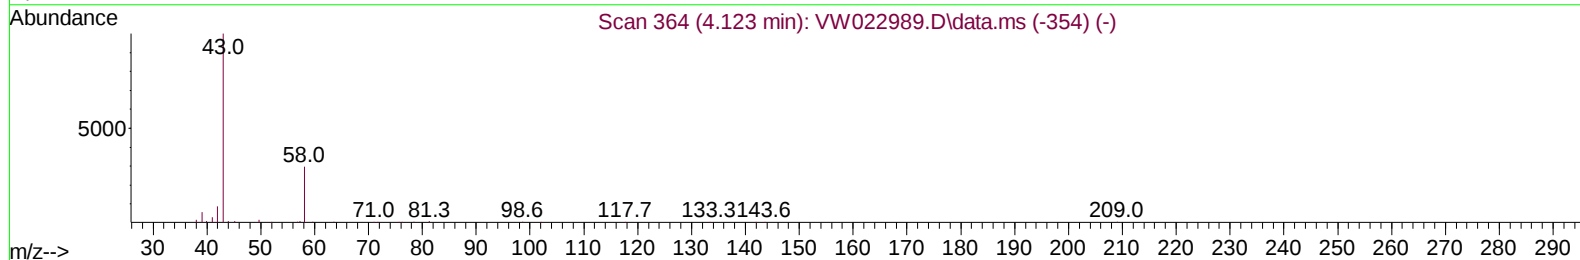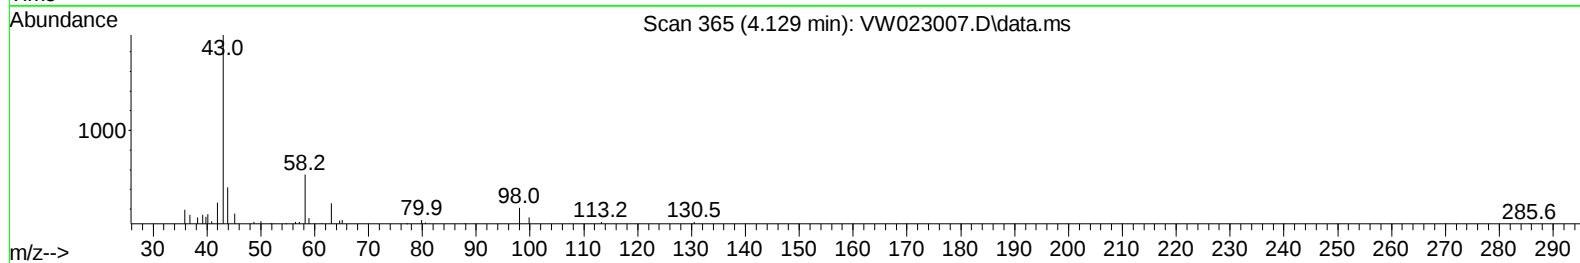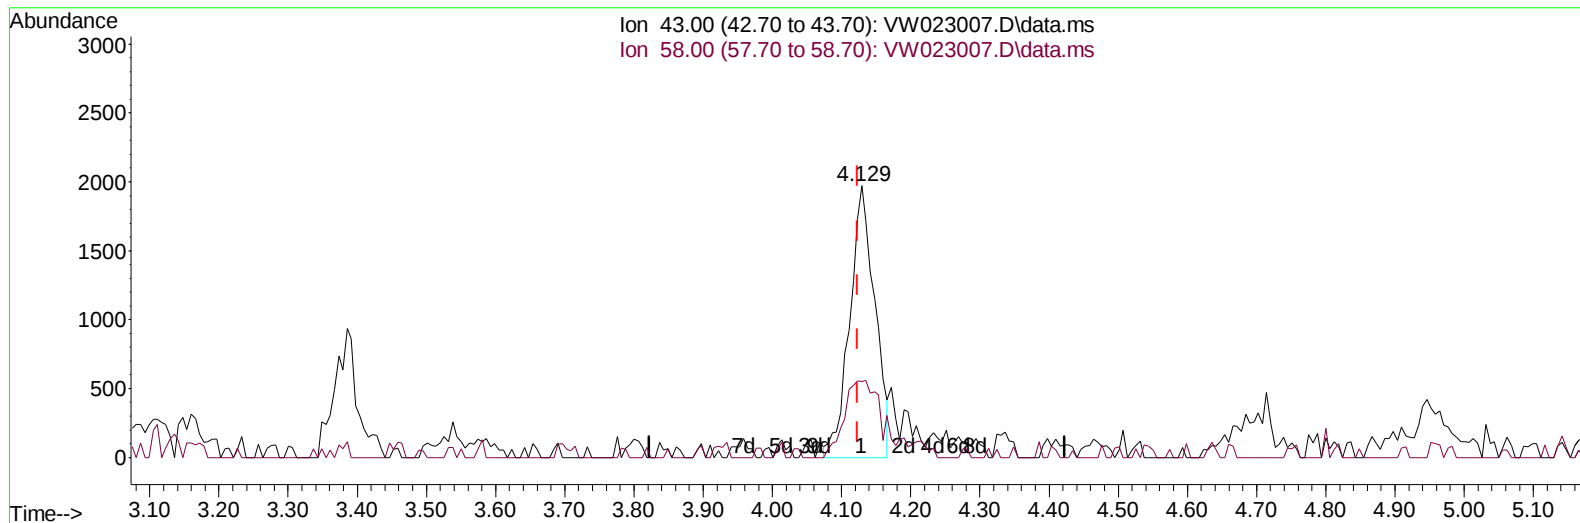

TIC: VW023007.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 5.29 ug/L

response 4975

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	28.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW023007.D
 Acq On : 12 May 2022 17:29
 Operator : SY/VA
 Sample : N2766-17
 Misc : 6.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4G7

Manual IntegrationsAPPROVED

Quant Time: May 13 01:13:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

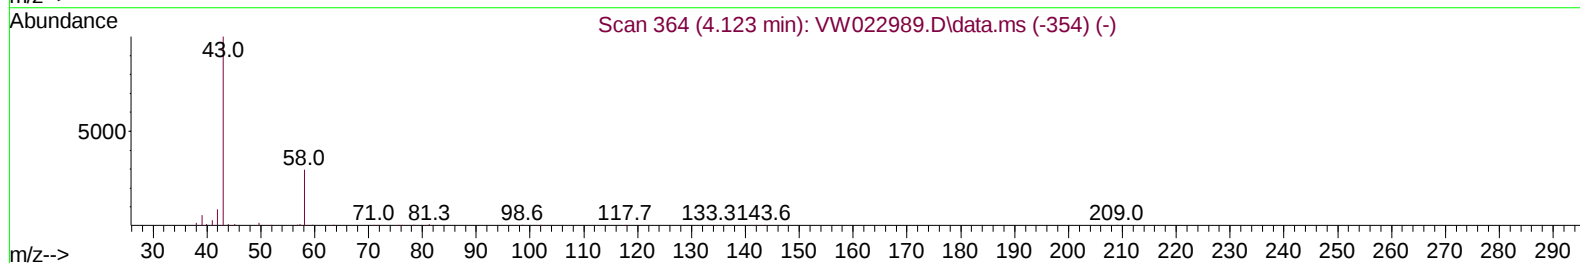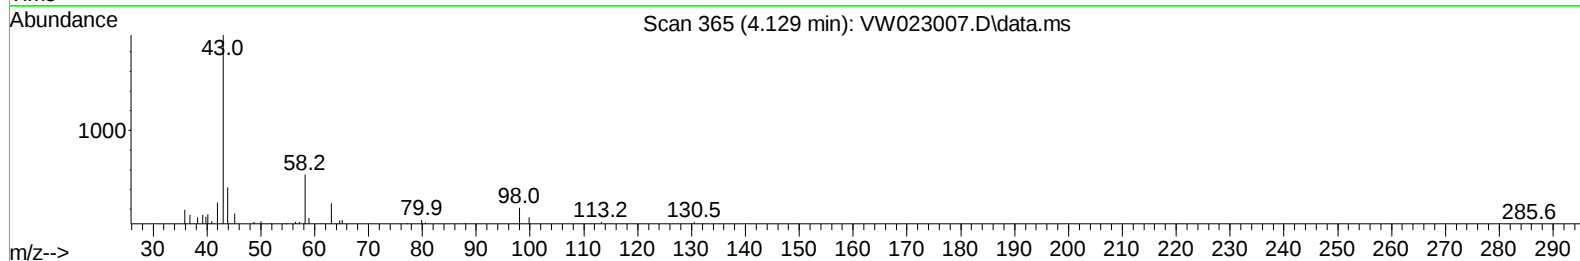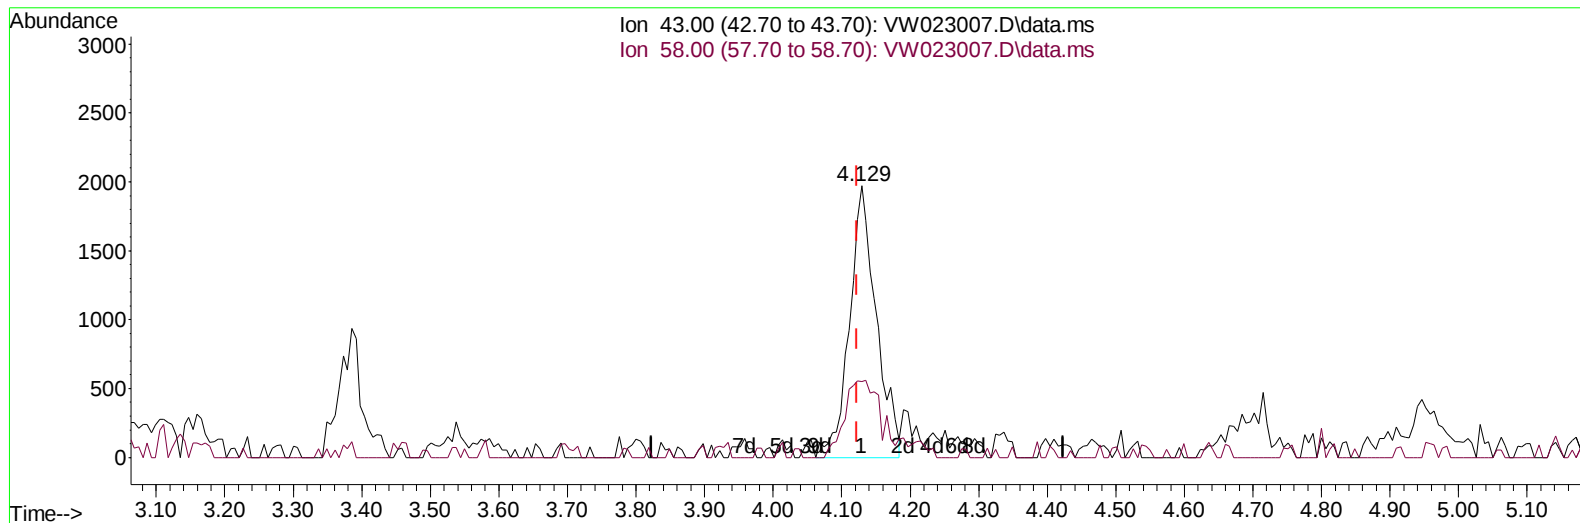

TIC: VW023007.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 5.72 ug/L m

response 5379

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	26.66
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW023007.D
 Acq On : 12 May 2022 17:29
 Operator : SY/VA
 Sample : N2766-17
 Misc : 6.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4G7

Manual IntegrationsAPPROVED

Quant Time: May 13 01:13:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		321981	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		285022	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		119766	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		107433	16.263	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	65.040%	
7) Chloroethane-d5	2.879	69		86433	20.112	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	80.440%	
11) 1,1-Dichloroethene-d2	4.013	63		105306	12.337	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	49.360%	
21) 2-Butanone-d5	7.074	46		67273	53.562	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	107.120%	
24) Chloroform-d	7.647	84		163310	17.312	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	69.240%	
26) 1,2-Dichloroethane-d4	8.305	65		115434	22.311	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	89.240%	
32) Benzene-d6	8.275	84		364874	22.210	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	88.840%	
36) 1,2-Dichloropropane-d6	9.275	67		115042	24.929	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	99.720%	
41) Toluene-d8	10.323	98		320649	20.205	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	80.800%	
43) trans-1,3-Dichloroprop...	10.579	79		42586	20.042	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	80.160%	
47) 2-Hexanone-d5	10.921	63		53232	60.425	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	120.860%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		66812	15.533	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	62.120%	
66) 1,2-Dichlorobenzene-d4	13.853	152		98019	23.412	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	93.640%	
Target Compounds							
13) Acetone	4.129	43		5379m	5.720	ug/L	
25) Chloroform	7.677	83		41680	4.792	ug/L	97
42) Toluene	10.390	91		20271	1.077	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
Data File : VW023007.D
Acq On : 12 May 2022 17:29
Operator : SY/VA
Sample : N2766-17
Misc : 6.88g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4G7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 13 01:13:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 01:10:05 2022
Response via : Initial Calibration

