

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
 Data File : VW022996.D
 Acq On : 12 May 2022 12:30
 Operator : SY/VA
 Sample : N2767-08
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 13 01:11:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 13 01:10:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	342558	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	332101	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	163758	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	98425	14.005	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.000%
7) Chloroethane-d5	2.885	69	86468	18.911	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.640%
11) 1,1-Dichloroethene-d2	4.013	63	107323	11.818	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	47.280%
21) 2-Butanone-d5	7.074	46	63768m	47.721	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.440%
24) Chloroform-d	7.653	84	207549	20.680	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.720%
26) 1,2-Dichloroethane-d4	8.305	65	119077	21.633	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.520%
32) Benzene-d6	8.275	84	378460	19.771	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.080%
36) 1,2-Dichloropropane-d6	9.274	67	117547	21.861	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.440%
41) Toluene-d8	10.323	98	349817	18.918	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.680%
43) trans-1,3-Dichloroprop...	10.579	79	46624	18.832	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.320%
47) 2-Hexanone-d5	10.921	63	48671	47.416	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.840%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	114143	22.775	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.080%
66) 1,2-Dichlorobenzene-d4	13.853	152	121032	21.143	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.560%
Target Compounds					Qvalue	
13) Acetone	4.117	43	4355m	4.353	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051222\
Data File : VW022996.D
Acq On : 12 May 2022 12:30
Operator : SY/VA
Sample : N2767-08
Misc : 5.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BGPM3

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 13 01:11:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 13 01:10:05 2022
Response via : Initial Calibration

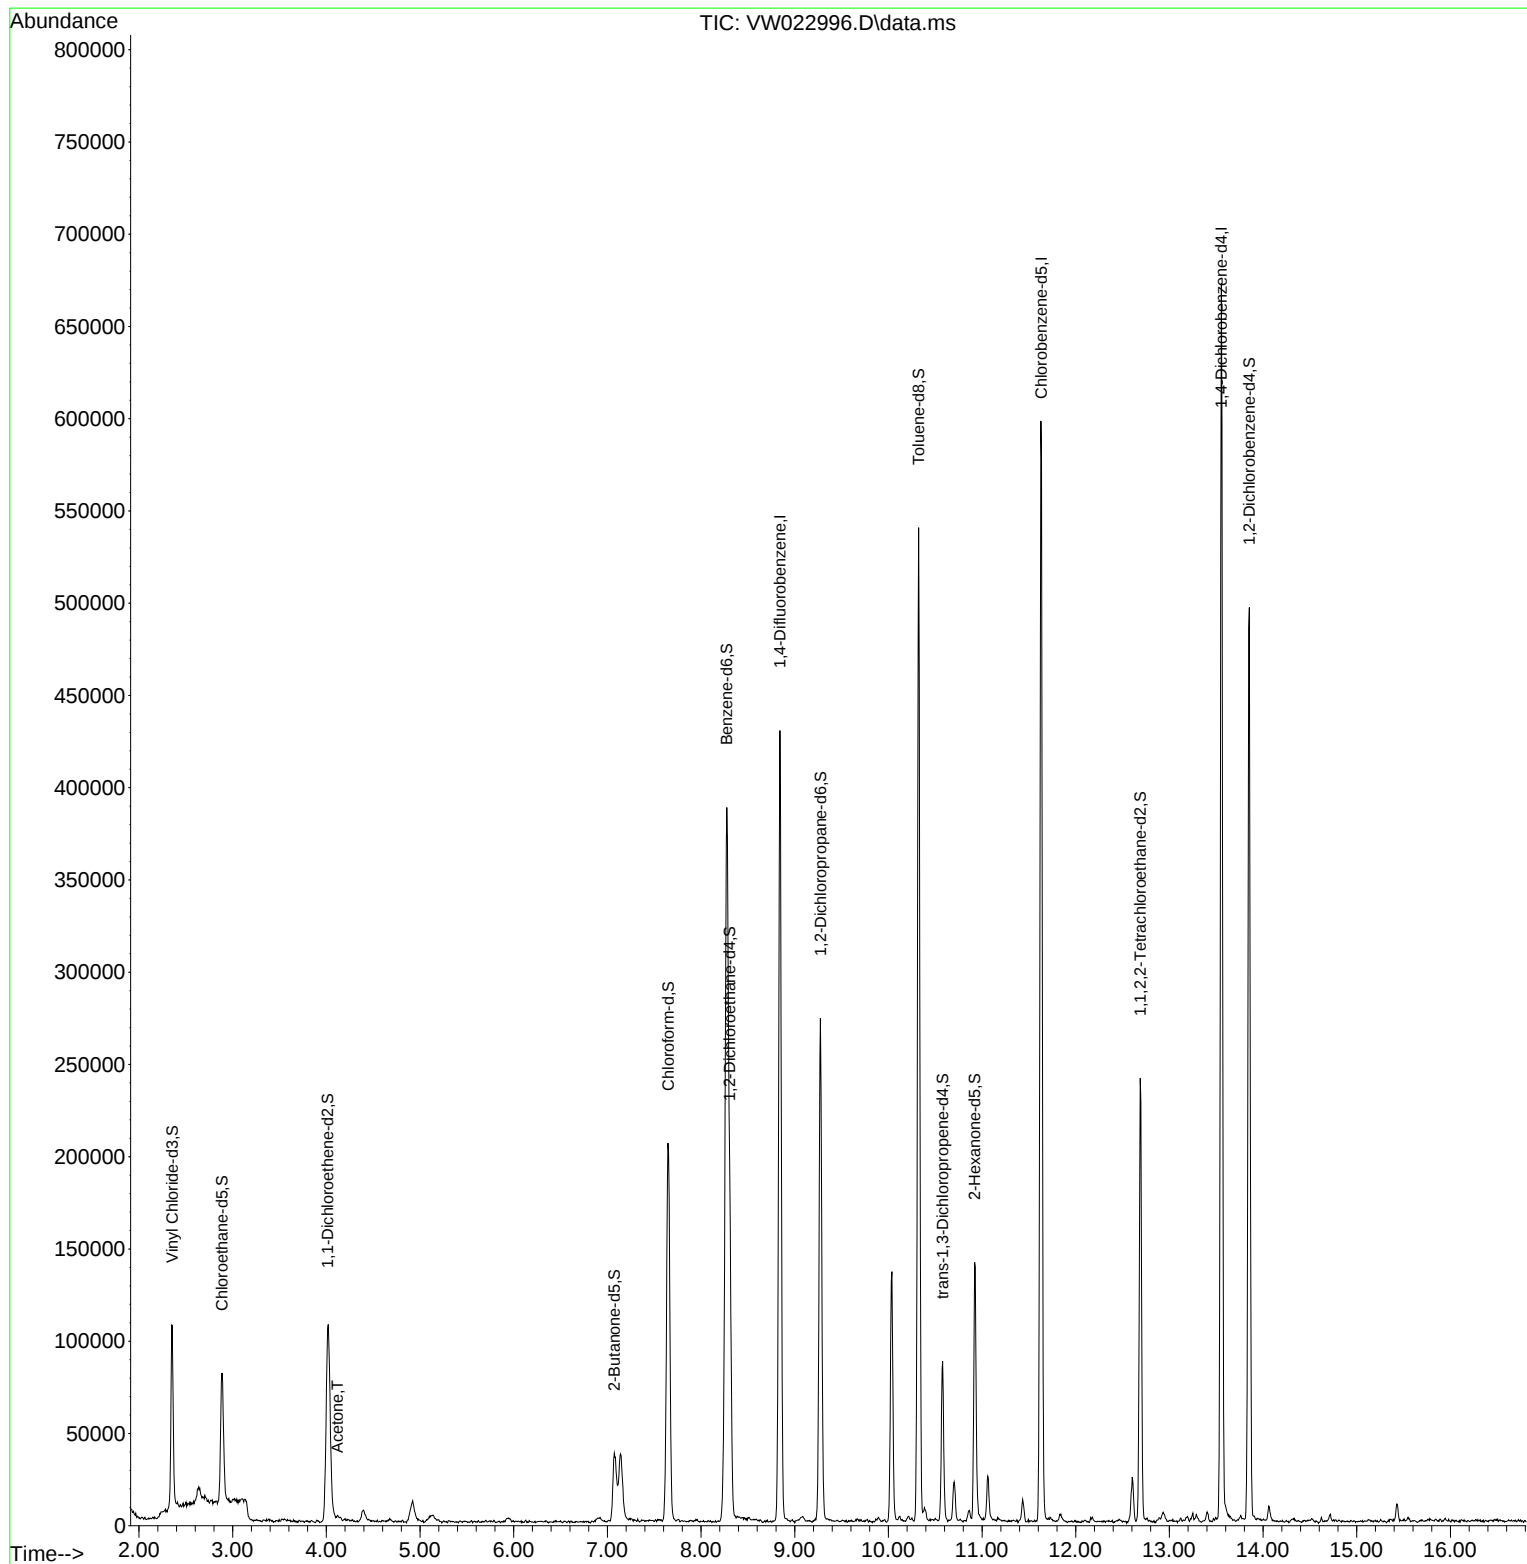

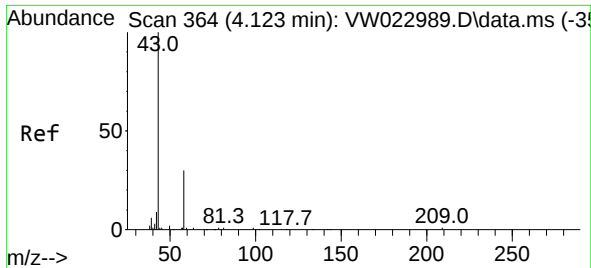

#13

Acetone

Concen: 4.353 ug/L m

RT: 4.117 min Scan# 30

Delta R.T. -0.006 min

Lab File: VW022996.D

Acq: 12 May 2022 12:30

Instrument :

MSVOA_W

ClientSampleId :

BGPM3

Tgt Ion: 43 Resp: 435

Ion Ratio Lower Upper

43 100

58 6.4 0.0 64.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/15/2022

Supervised By :Mahesh Dadoda 05/16/2022

